


Yusuf Miah 1 cat.b P
P31CPD.qm CDC13 /opt/data Adv_Exp 13

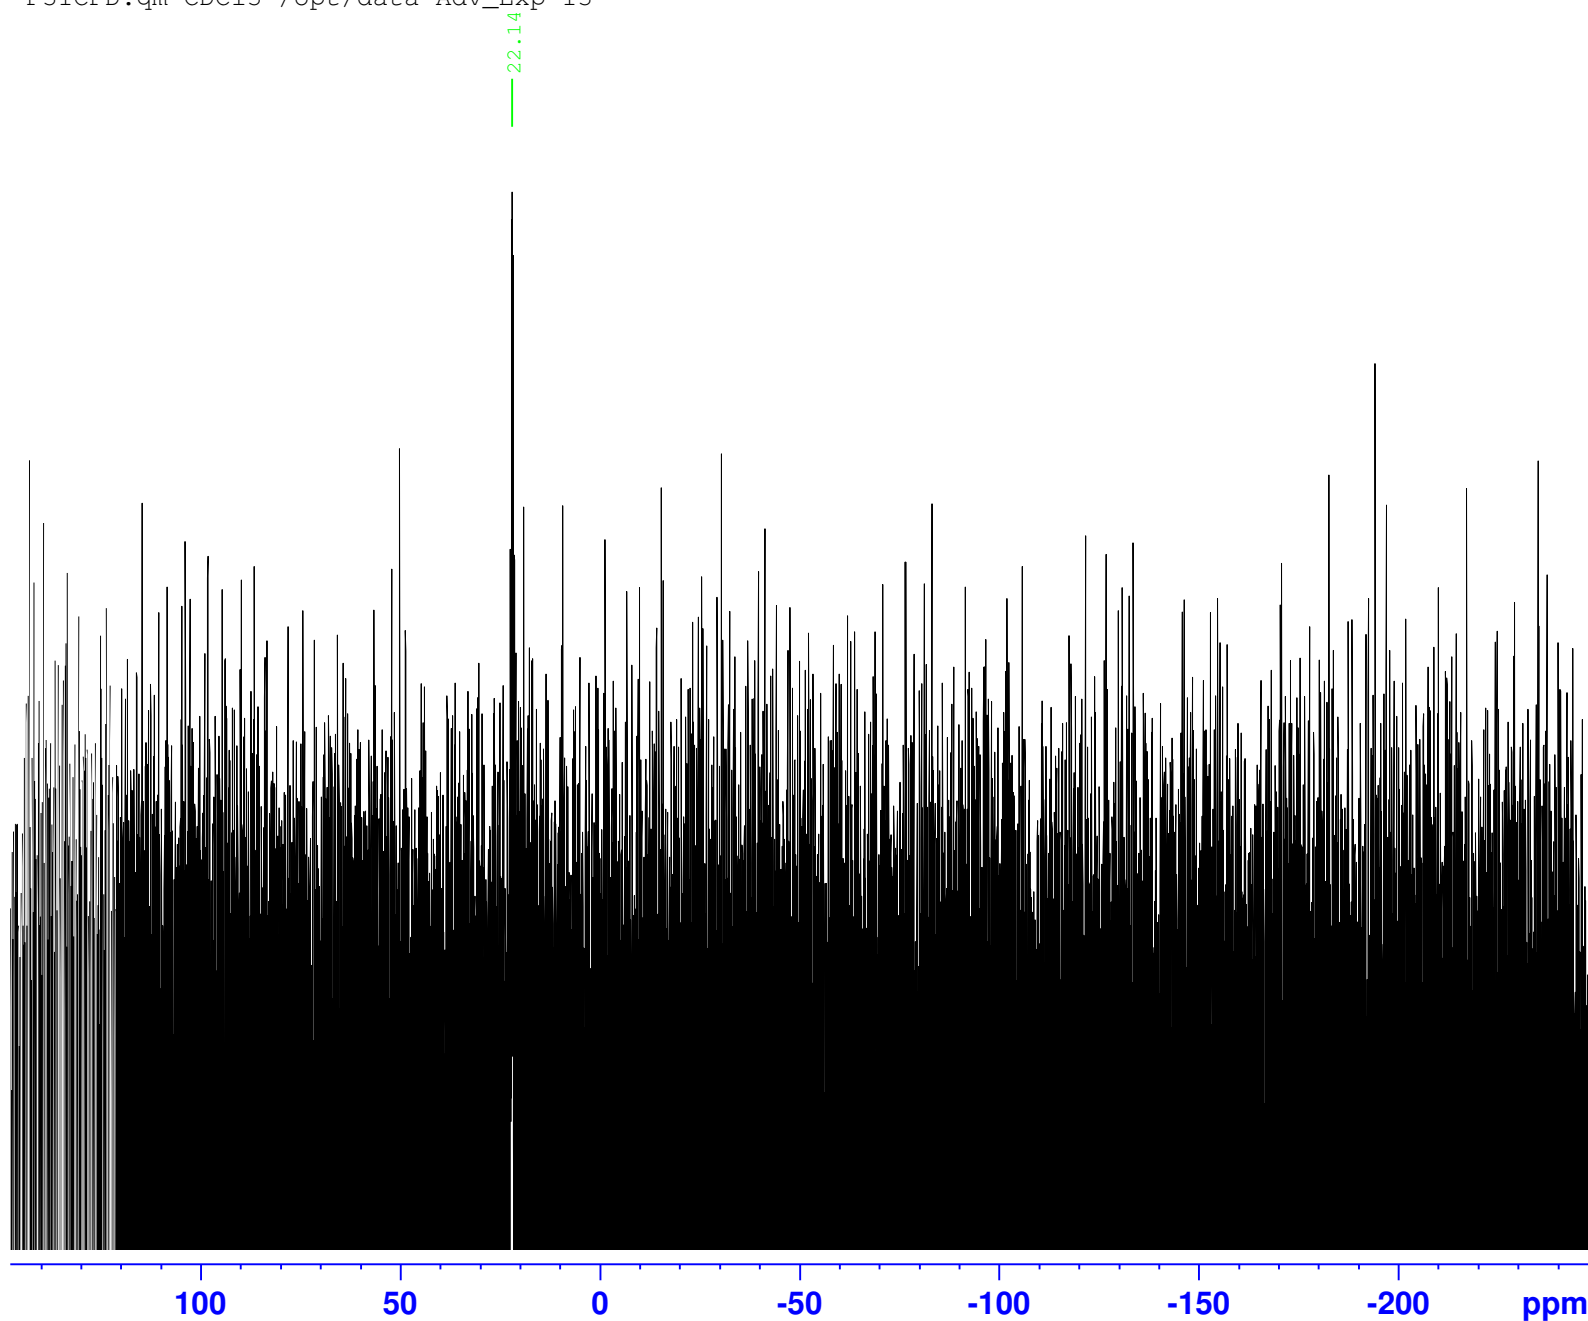

Current Data Parameters
NAME X_160223
EXPNO 212
PROCNO 1

F2 - Acquisition Parameters
Date_ 20160223
Time 19.07
INSTRUM aviii400
PROBHD 5 mm PABBO BB-
PULPROG zgig
TD 128198
SOLVENT CDC13
NS 32
DS 2
SWH 64102.562 Hz
FIDRES 0.500028 Hz
AQ 0.9999444 sec
RG 1620
DW 7.800 usec
DE 7.13 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 161.9958293 MHz
NUC1 31P
P1 11.30 usec
PLW1 19.05500031 W

===== CHANNEL f2 =====
SFO2 400.2024012 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 12.58899975 W
PLW12 0.26631001 W

F2 - Processing parameters
SI 262144
SF 162.0039290 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

0.21 1.93 0.20 1.36 0.81 1.32 0.51 0.84 7.06 9.89 7.89 1.77 0.48 0.06 1.39 1.23 0.61 0.24 0.78 0.67 0.57 0.26 3.24 1.05 0.78 0.66 1.01 0.30 0.83 0.58 0.29 0.40 0.15 2.11 0.21 1.21 1.37 0.26 0.13 1.39 1.79 1.33 1.61 0.94 0.14 0.49 2.07 0.20 0.21