


CoupledProduct-PdCatB-MT
P31CPD.qm CDC13 /opt/data Adv_Exp 10

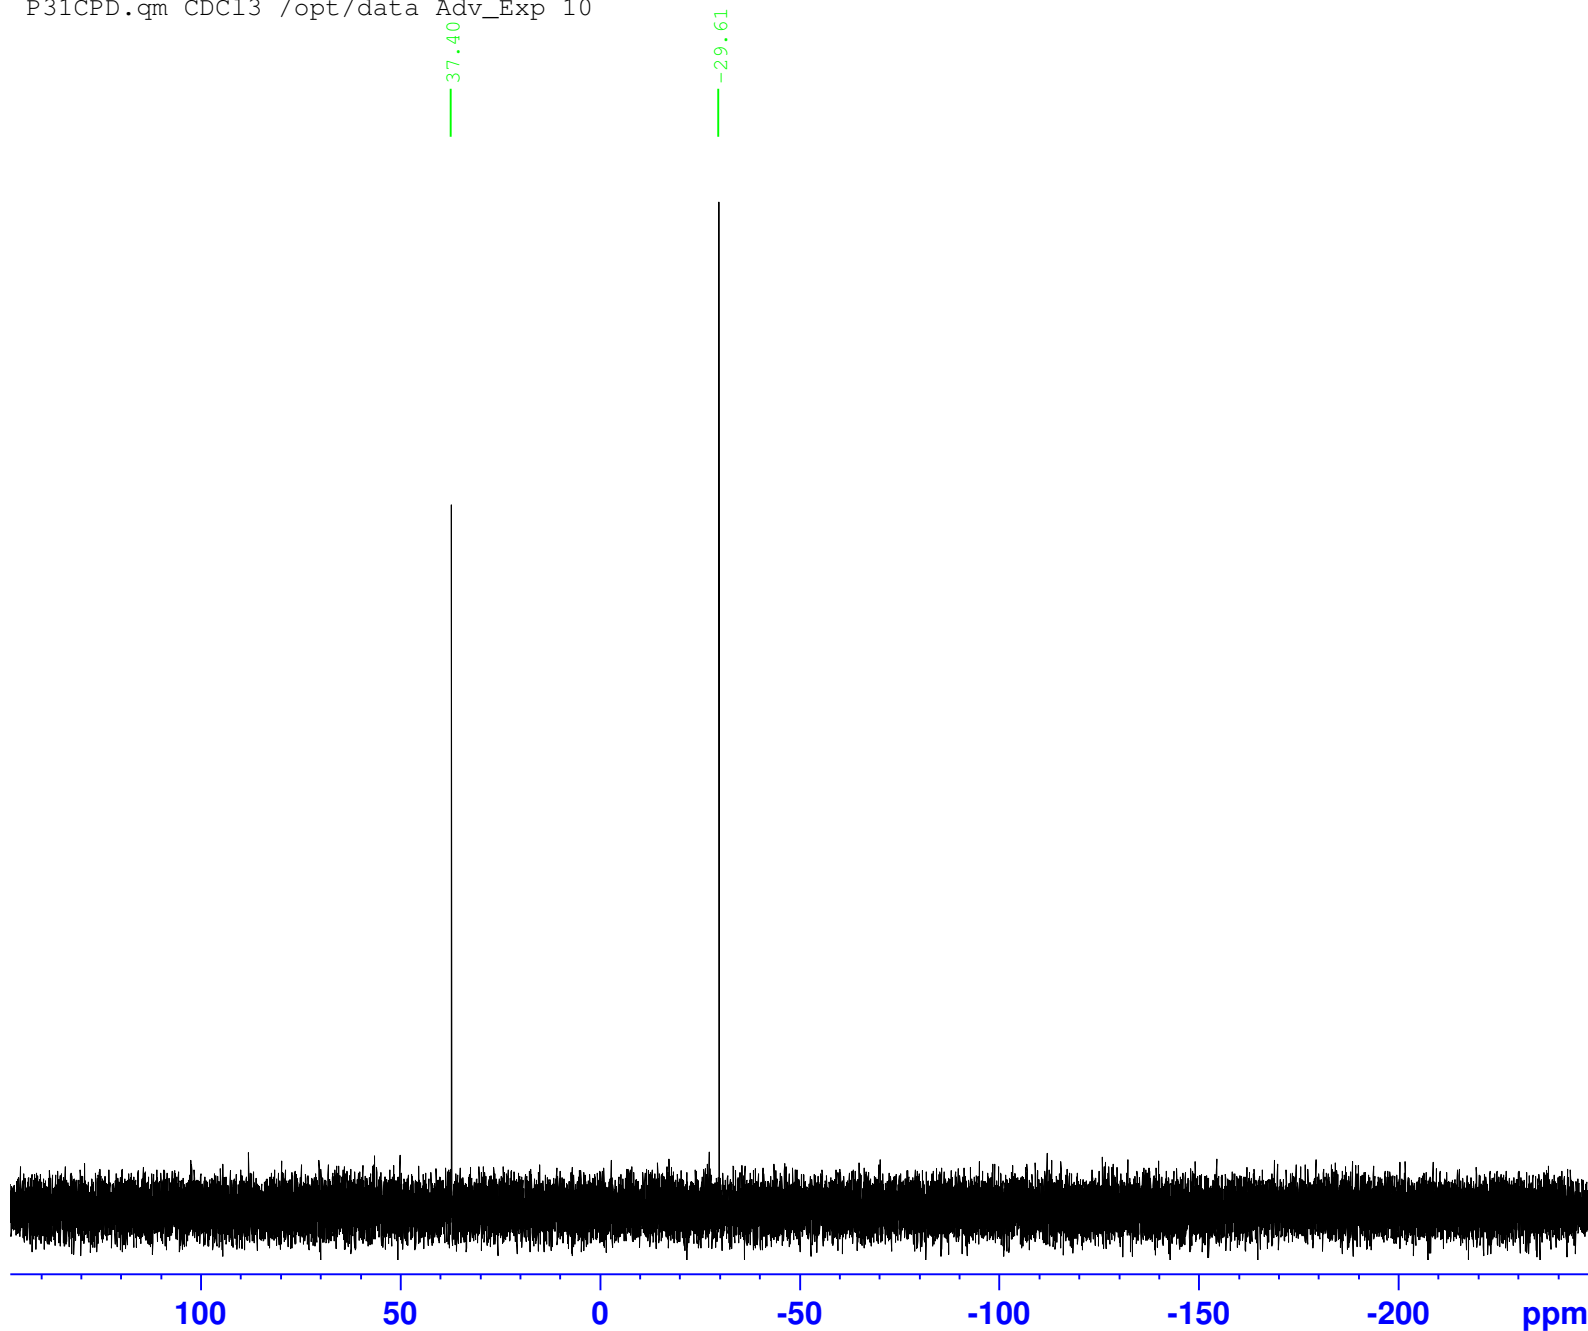

Current Data Parameters
NAME X_160225
EXPNO 212
PROCNO 1

F2 - Acquisition Parameters
Date_ 20160225
Time 14.01
INSTRUM aviii400
PROBHD 5 mm PABBO BB-
PULPROG zgig
TD 128198
SOLVENT CDC13
NS 32
DS 2
SWH 64102.562 Hz
FIDRES 0.500028 Hz
AQ 0.9999444 sec
RG 2050
DW 7.800 usec
DE 7.13 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 161.9958293 MHz
NUC1 31P
P1 11.30 usec
PLW1 19.05500031 W

===== CHANNEL f2 =====
SFO2 400.2024012 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 12.58899975 W
PLW12 0.26631001 W

F2 - Processing parameters
SI 262144
SF 162.0039290 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

0.13
1.55
1.14
0.39
0.79
1.39
0.52
0.89
0.26
0.69
1.51
1.66
0.29
0.91
1.54
0.60
2.65
0.04
1.37
1.07
0.98
1.74
0.29
1.52
0.86
1.48
1.41
1.72
1.32
1.35
0.94
0.92
0.25
0.46
1.95
0.93
2.01
0.87
0.51
1.50
1.00
0.47
2.95
0.82
0.87
1.45
0.97
0.89
1.19