


SEH Pdcl2pph3 31P
P31CPD.qm CDC13 /opt/data Adv_Exp 38

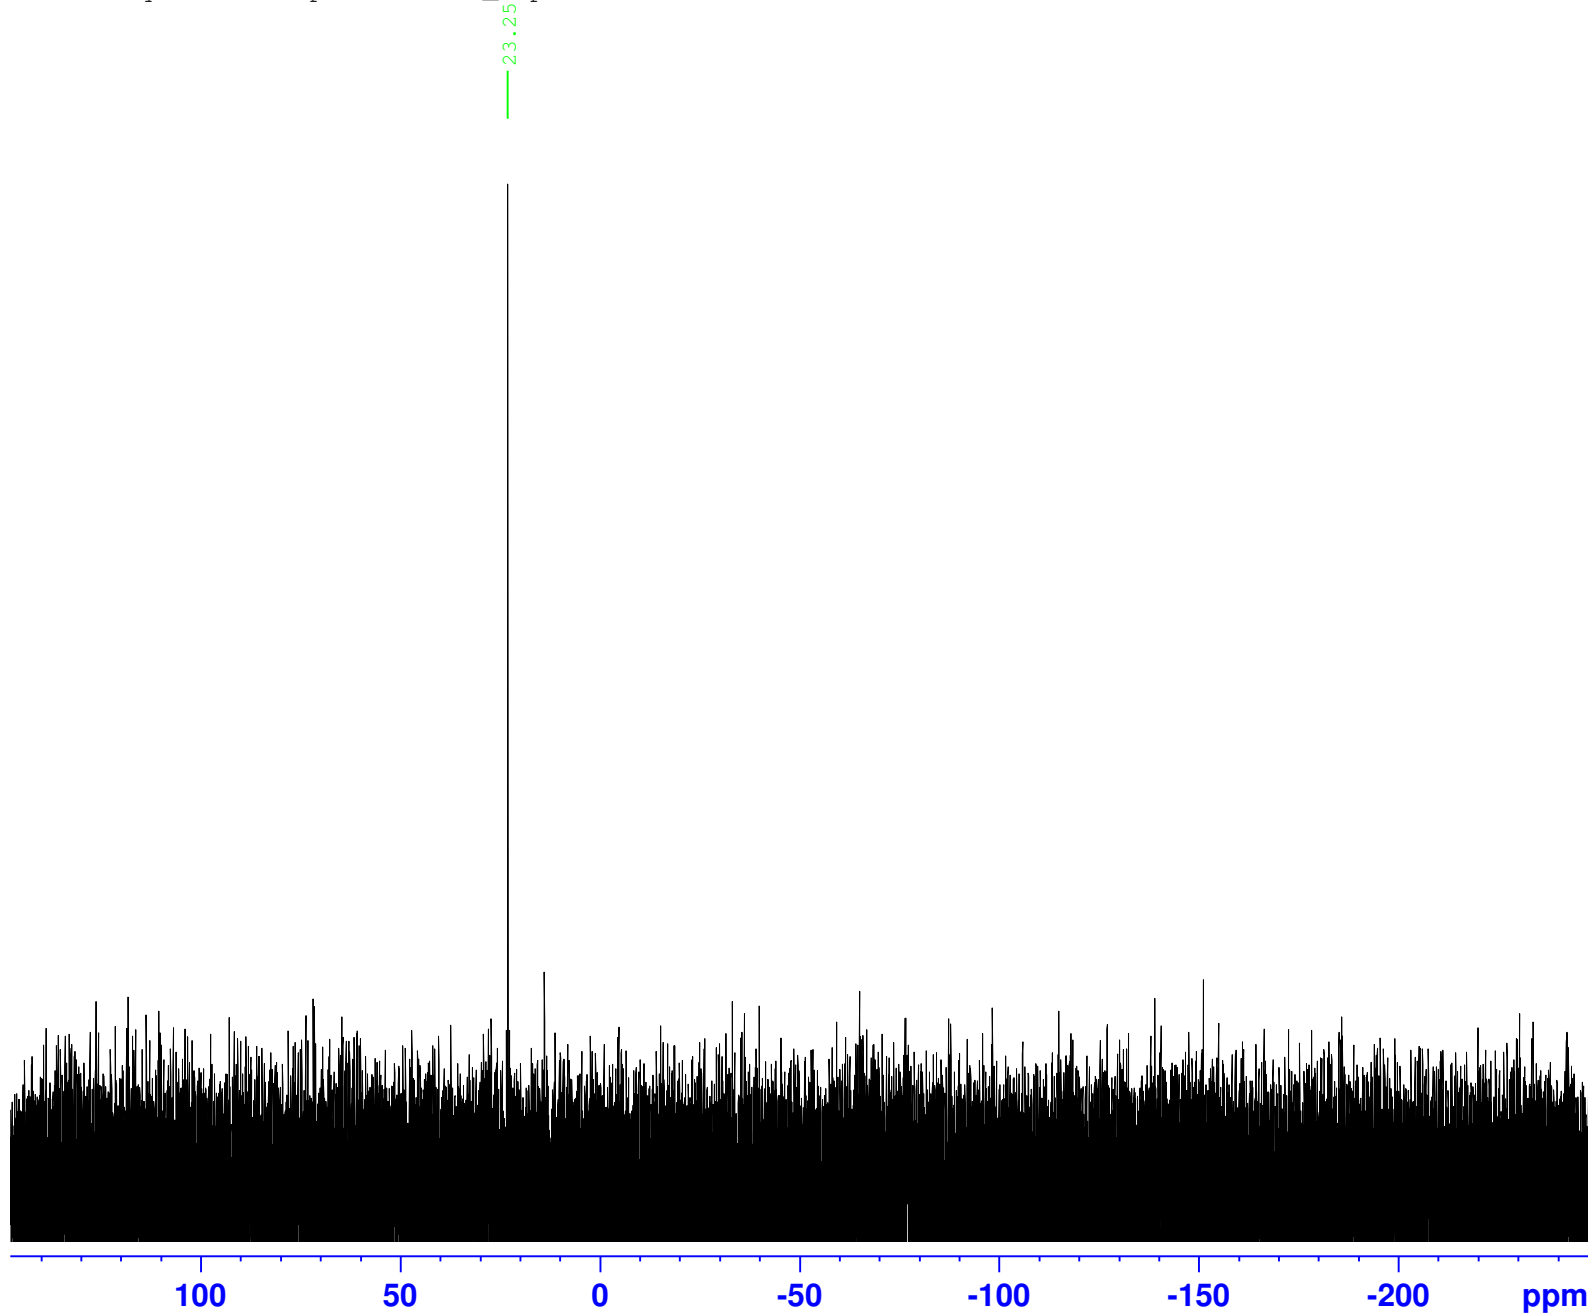

Current Data Parameters
NAME X_160927
EXPNO 562
PROCNO 1

F2 - Acquisition Parameters
Date_ 20160927
Time 15.04
INSTRUM aviii400
PROBHD 5 mm PABBO BB-
PULPROG zgig
TD 128198
SOLVENT CDC13
NS 32
DS 2
SWH 64102.562 Hz
FIDRES 0.500028 Hz
AQ 0.9999444 sec
RG 1620
DW 7.800 usec
DE 7.13 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 161.9958293 MHz
NUC1 31P
P1 11.30 usec
PLW1 19.05500031 W

===== CHANNEL f2 =====
SFO2 400.2024012 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 12.58899975 W
PLW12 0.26631001 W

F2 - Processing parameters
SI 262144
SF 162.0039290 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

0.33 0.18 0.18 2.19 1.44 0.78 0.34 1.50 1.46 1.67 0.35 5.76 0.75 1.59 0.28 0.92 0.84 0.64 1.66 0.01 1.79 0.18 0.72 0.02 0.05 0.41 1.90 1.74 0.81 1.40 0.84 1.30 1.05 1.32 0.38 0.57 0.25 1.68 1.68 1.39 1.85 1.13 0.13 0.34 1.22 0.17 2.81