


SEH analogue pure 31P B3P  
P31CPD.qm CDC13 /opt/data Adv\_Exp 9

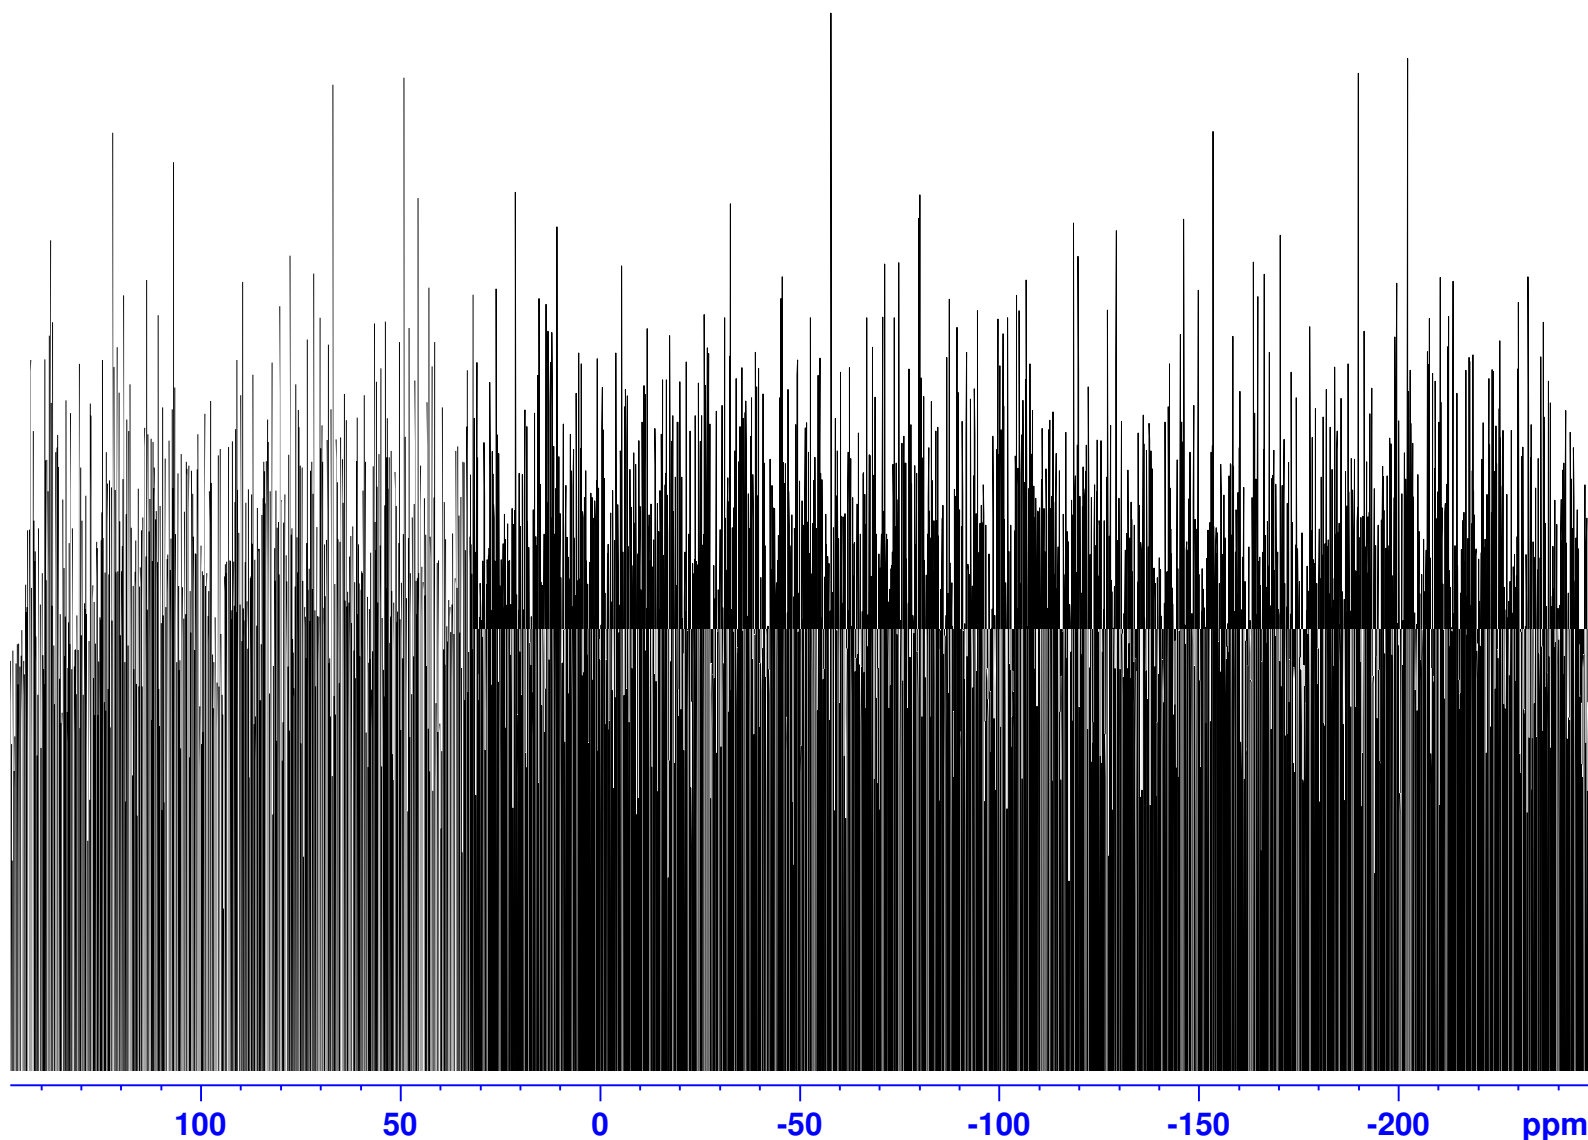

#### Current Data Parameters

NAME X\_160929  
EXPNO 252  
PROCNO 1

#### F2 - Acquisition Parameters

Date\_ 20160929  
Time 17.03  
INSTRUM aviii400  
PROBHD 5 mm PABBO BB-  
PULPROG zgig  
TD 128198  
SOLVENT CDC13  
NS 32  
DS 2  
SWH 64102.562 Hz  
FIDRES 0.500028 Hz  
AQ 0.9999444 sec  
RG 1820  
DW 7.800 usec  
DE 7.13 usec  
TE 300.0 K  
D1 2.00000000 sec  
D11 0.03000000 sec  
TD0 1

#### ===== CHANNEL f1 =====

SFO1 161.9958293 MHz  
NUC1 31P  
P1 11.30 usec  
PLW1 19.05500031 W

#### ===== CHANNEL f2 =====

SFO2 400.2024012 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 12.58899975 W  
PLW12 0.26631001 W

#### F2 - Processing parameters

SI 262144  
SF 162.0039290 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40

0.95  
0.25  
0.26  
1.24  
0.16  
0.45  
0.47  
0.57  
0.84  
1.07  
1.62  
0.37  
1.20  
1.22  
0.59  
1.53  
0.70  
0.16  
2.02  
0.29  
1.01  
1.60  
0.15  
2.01  
0.49  
3.41  
0.34  
0.72  
1.07  
0.47  
1.57  
1.06  
0.88  
0.50  
1.08  
1.11  
0.15  
0.52  
1.96  
2.17  
0.03  
1.27  
2.16  
0.90  
0.86  
1.22  
1.18  
2.23