


npp2 product 2
P31CPD.qm CDC13 /opt/data Adv_Exp 28

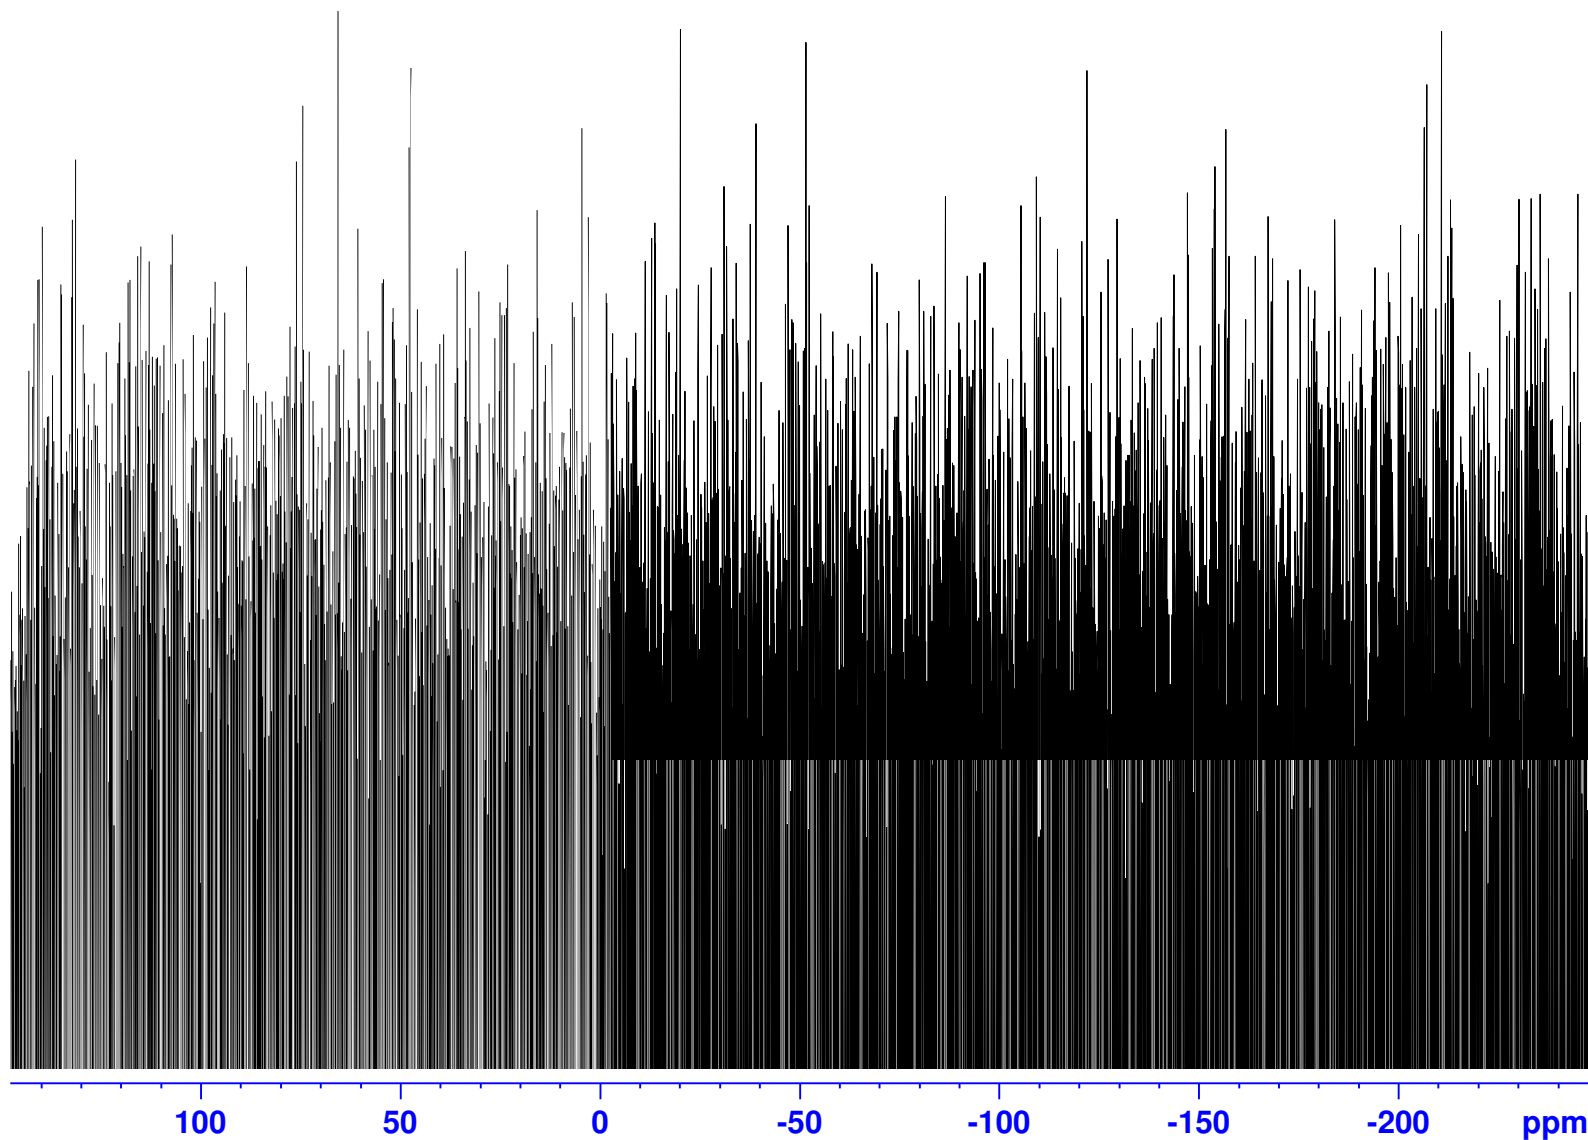

Current Data Parameters
NAME X_160929
EXPNO 352
PROCNO 1

F2 - Acquisition Parameters
Date_ 20160930
Time 3.55
INSTRUM aviii400
PROBHD 5 mm PABBO BB-
PULPROG zgig
TD 128198
SOLVENT CDC13
NS 32
DS 2
SWH 64102.562 Hz
FIDRES 0.500028 Hz
AQ 0.9999444 sec
RG 2050
DW 7.800 usec
DE 7.13 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 161.9958293 MHz
NUC1 31P
P1 11.30 usec
PLW1 19.05500031 W

===== CHANNEL f2 =====
SFO2 400.2024012 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 12.58899975 W
PLW12 0.26631001 W

F2 - Processing parameters
SI 262144
SF 162.0039290 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

0.32 0.19 0.29 1.42 2.00 0.93 0.92 1.09 0.03 0.42 1.95 3.14 1.19 0.49 1.13 0.32 0.14 0.34 1.19 0.89 0.12 0.12 1.17 1.08 1.42 2.06 1.22 0.97 0.75 1.37 0.60 0.78 1.43 1.14 0.77 0.32 1.36 0.05 0.61 2.60 0.74 1.36 0.59 1.26 2.70 1.67 0.53 1.96 1.85