


Reflux product 1 - Sabiha Patel
P31CPD.qm CDC13 /opt/data Adv_Exp 12

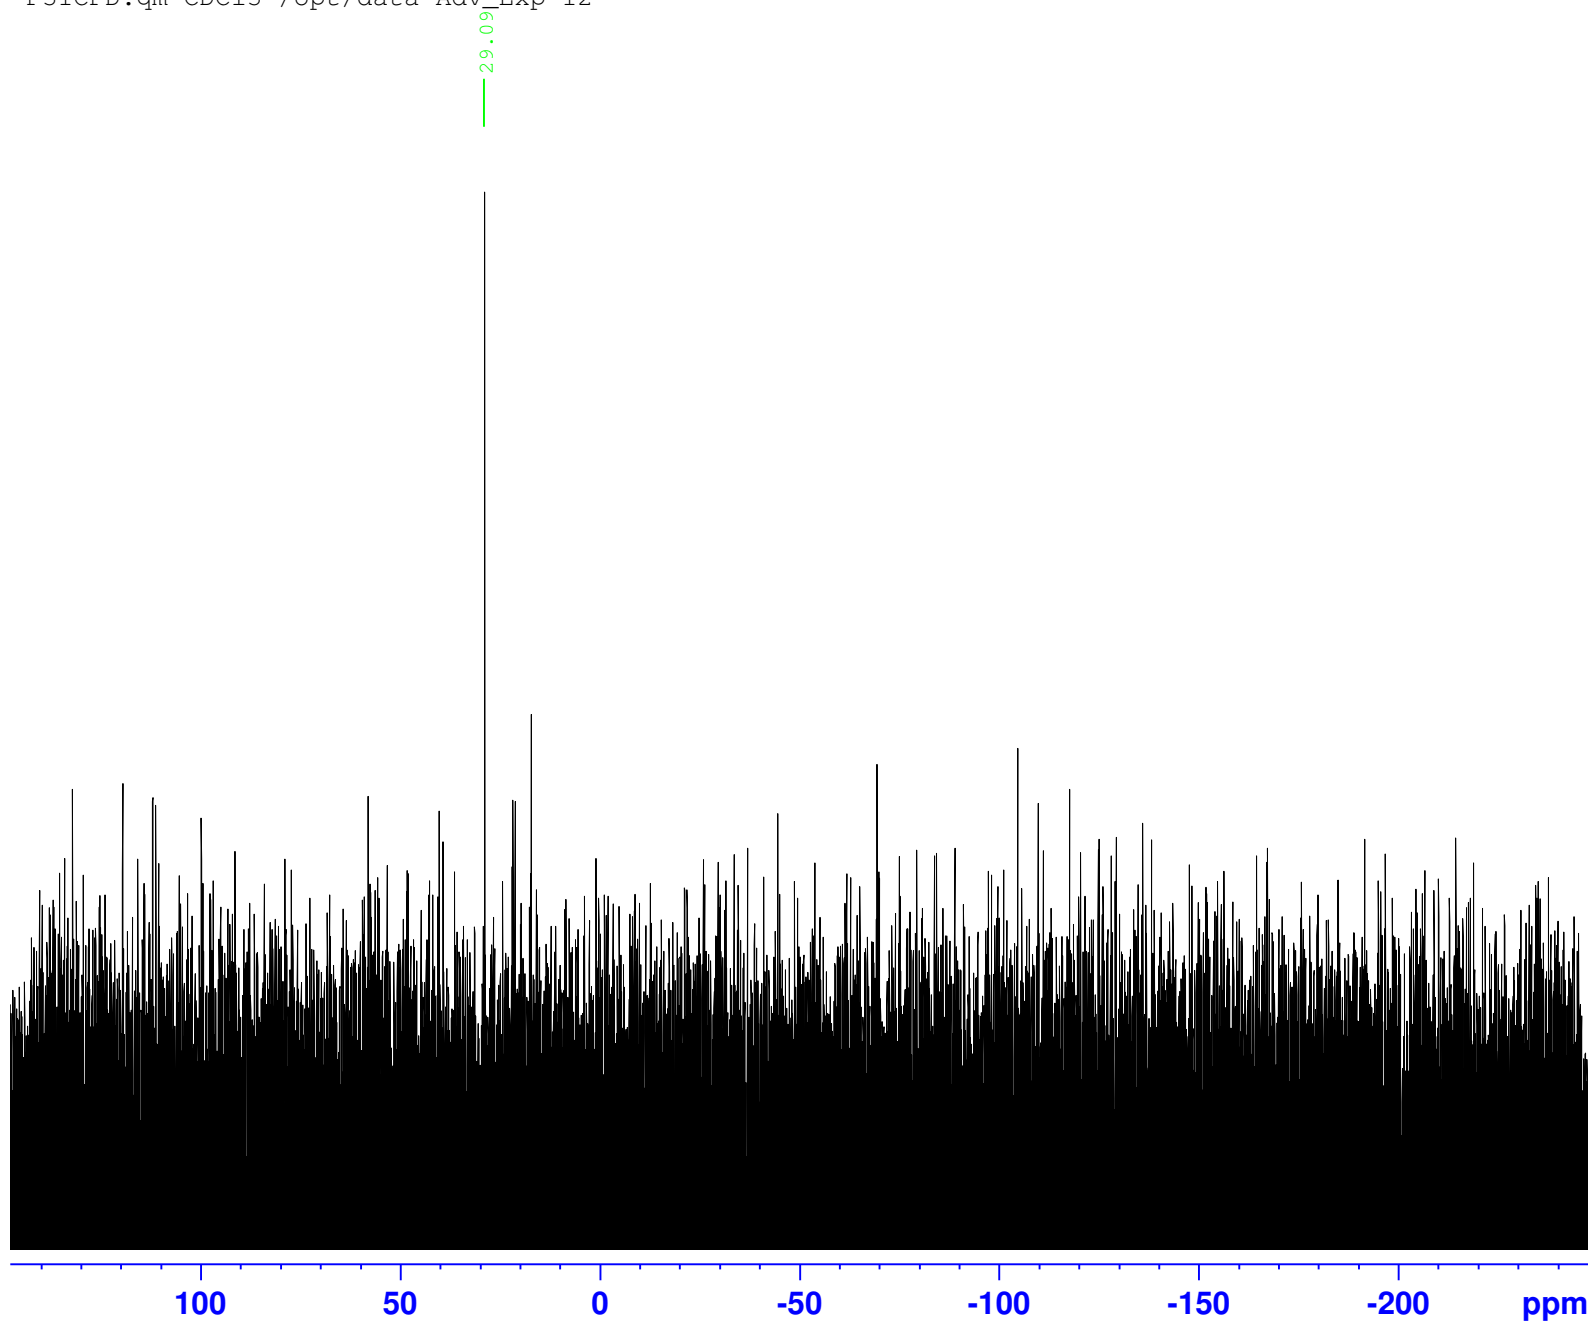

Current Data Parameters
NAME X_160930
EXPNO 32
PROCNO 1

F2 - Acquisition Parameters
Date_ 20160930
Time 10.34
INSTRUM aviii400
PROBHD 5 mm PABBO BB-
PULPROG zgig
TD 128198
SOLVENT CDC13
NS 32
DS 2
SWH 64102.562 Hz
FIDRES 0.500028 Hz
AQ 0.9999444 sec
RG 2050
DW 7.800 usec
DE 7.13 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 161.9958293 MHz
NUC1 31P
P1 11.30 usec
PLW1 19.05500031 W

===== CHANNEL f2 =====
SFO2 400.2024012 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 12.58899975 W
PLW12 0.26631001 W

F2 - Processing parameters
SI 262144
SF 162.0039290 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

0.20 2.72 0.53 1.10 0.78 2.30 2.00 0.94 0.81 1.31 0.09 3.85 1.83 2.65 1.11 1.18 0.00 1.41 1.28 3.24 0.87 1.71 1.20 0.41 0.73 1.69 1.14 0.76 1.18 0.61 0.09 1.85 1.02 0.40 2.00 1.34 0.14 0.48 1.53 1.23 0.14 0.37 1.18 0.37 4.62 0.13 0.40 1.52 0.50