


Refluc product 1 - Ismahan Moalin
P31CPD.qm CDC13 /opt/data Adv_Exp 18

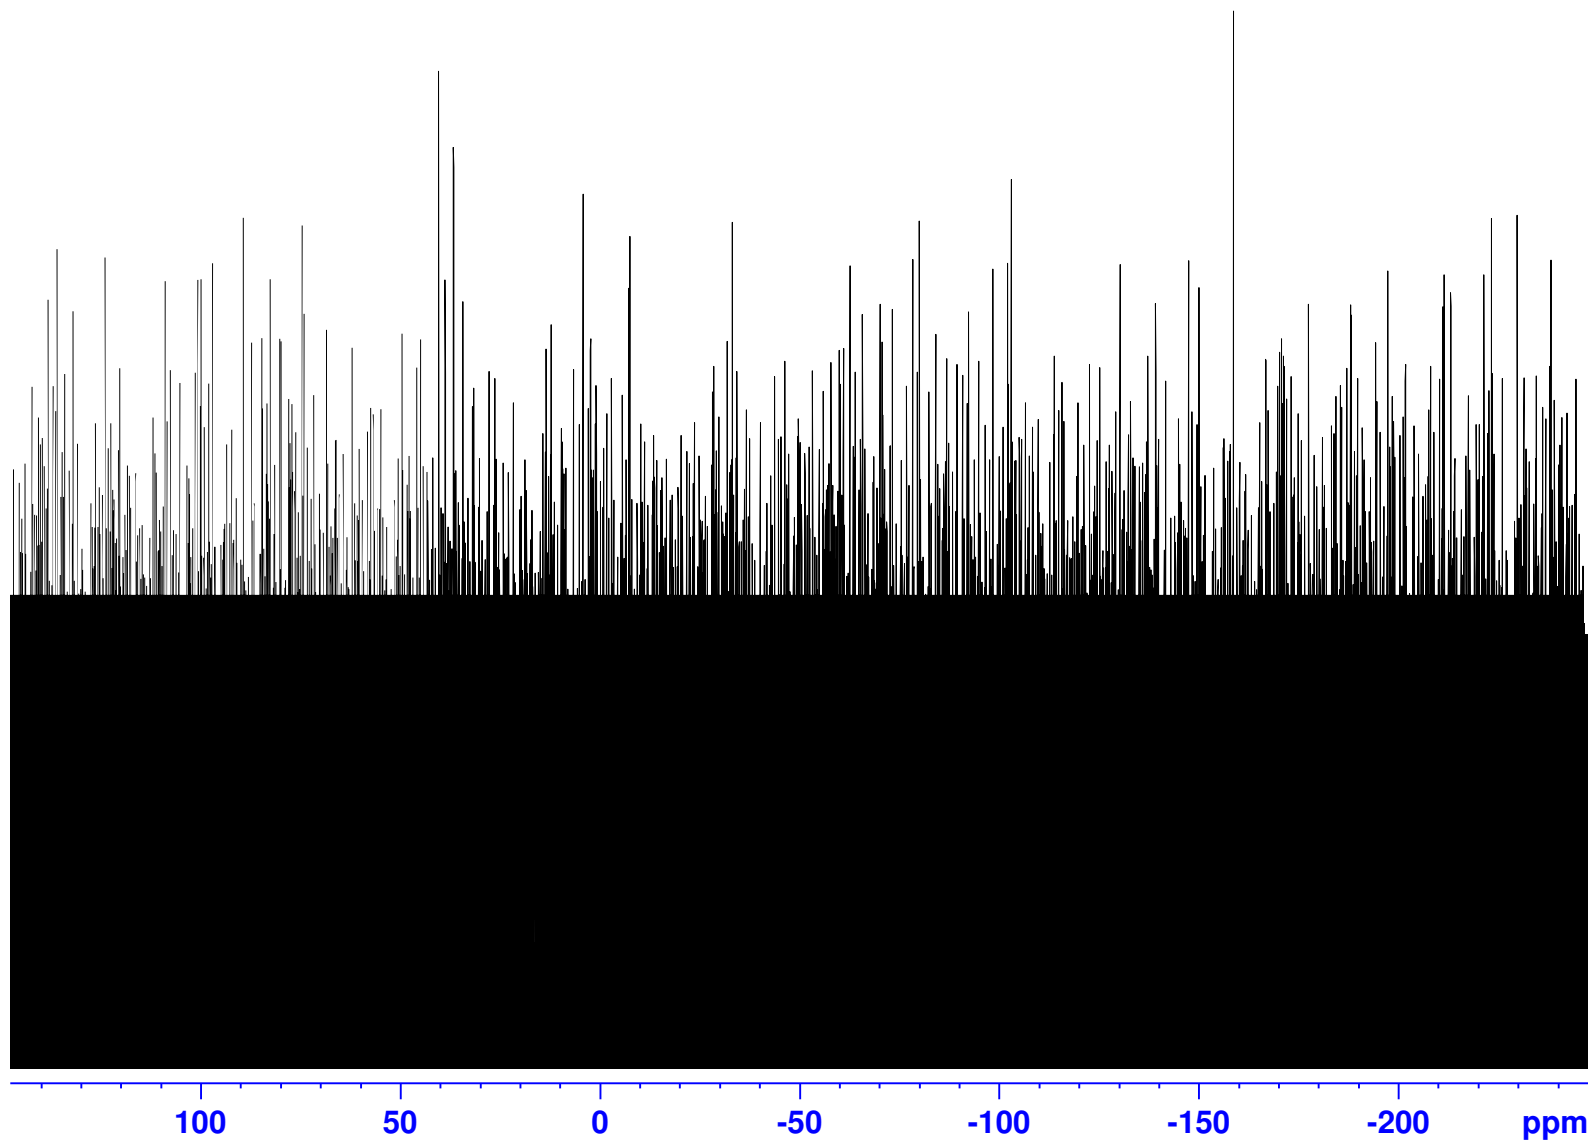

Current Data Parameters
NAME X_160930
EXPNO 92
PROCNO 1

F2 - Acquisition Parameters
Date_ 20160930
Time 12.45
INSTRUM aviii400
PROBHD 5 mm PABBO BB-
PULPROG zgig
TD 128198
SOLVENT CDC13
NS 32
DS 2
SWH 64102.562 Hz
FIDRES 0.500028 Hz
AQ 0.9999444 sec
RG 1620
DW 7.800 usec
DE 7.13 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 161.9958293 MHz
NUC1 31P
P1 11.30 usec
PLW1 19.05500031 W

===== CHANNEL f2 =====
SFO2 400.2024012 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 12.58899975 W
PLW12 0.26631001 W

F2 - Processing parameters
SI 262144
SF 162.0039290 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

0.39 1.46 2.39 1.86 2.04 1.24 0.38 0.82 2.28 0.48 1.81 2.22 0.15 1.13 1.61 0.89 1.70 0.93 1.11 2.68 0.69 1.16 0.13 3.07 0.99 1.16 2.07 1.50 1.78 1.01 1.18 0.42 1.68 0.50 1.70 0.70 2.21 0.97 0.62 1.37 1.24 0.98 0.29 1.28 3.29 0.45 1.19 0.73 1.84