

2016-09-19 - 440

C NMR

CDC13

C13CPD256 CDC13 /opt/data/Adv Exp 44




191.18  
149.46  
146.95  
135.56  
129.01  
128.00  
126.11  
116.37  
107.06

77.40  
77.08  
76.77

56.25  
56.24

33.47  
31.57

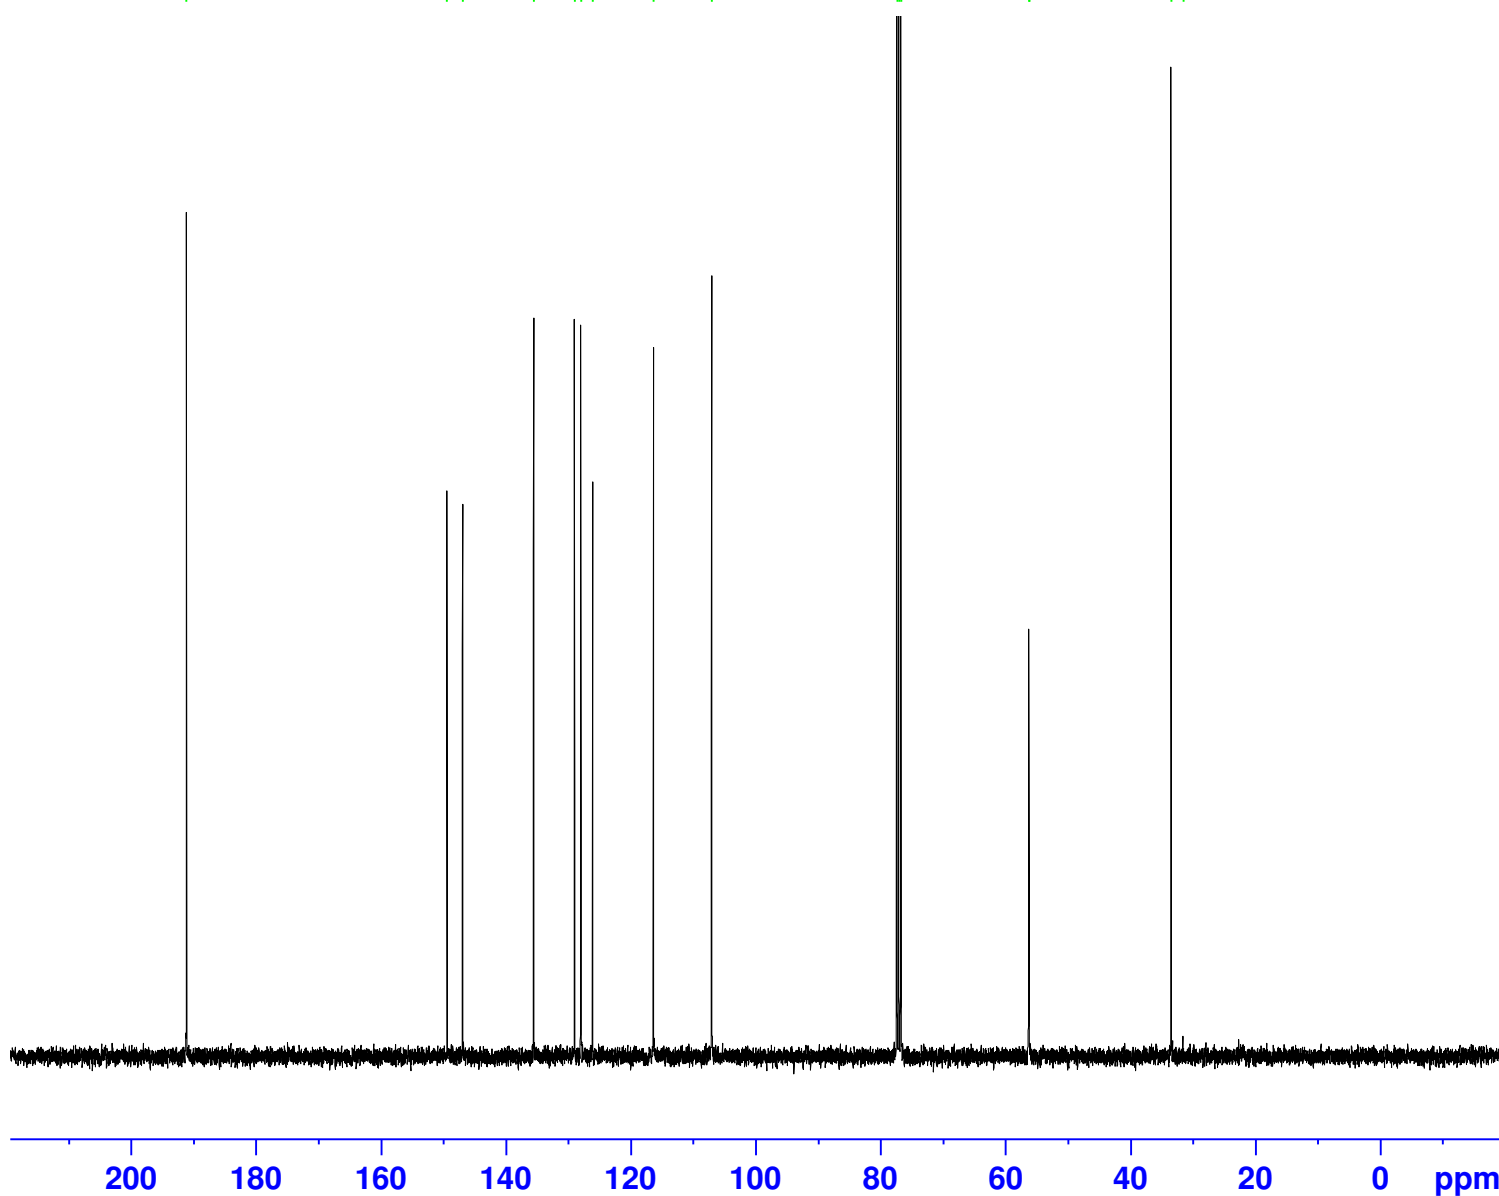

Current Data Parameters  
NAME X\_161004  
EXPNO 441  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20161004  
Time 23.09  
INSTRUM aviii400  
PROBHD 5 mm PABBO BB-  
PULPROG zgpg30  
TD 65536  
SOLVENT CDC13  
NS 256  
DS 4  
SWH 24038.461 Hz  
FIDRES 0.366798 Hz  
AQ 1.3631488 sec  
RG 1820  
DW 20.800 usec  
DE 6.50 usec  
TE 300.0 K  
D1 2.00000000 sec  
D11 0.03000000 sec  
TD0 1

===== CHANNEL f1 =====  
SFO1 100.6404326 MHz  
NUC1 13C  
P1 9.00 usec  
PLW1 50.11899948 W

===== CHANNEL f2 =====  
SFO2 400.2016008 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 12.58899975 W  
PLW12 0.26631001 W  
PLW13 0.21571000 W

F2 - Processing parameters  
SI 32768  
SF 100.6303700 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40