


2016 - 11 - 07 - 310

¹H NMR

CDCl₃

PROTON.qm CDCl₃ /opt/data Adv_Exp 1

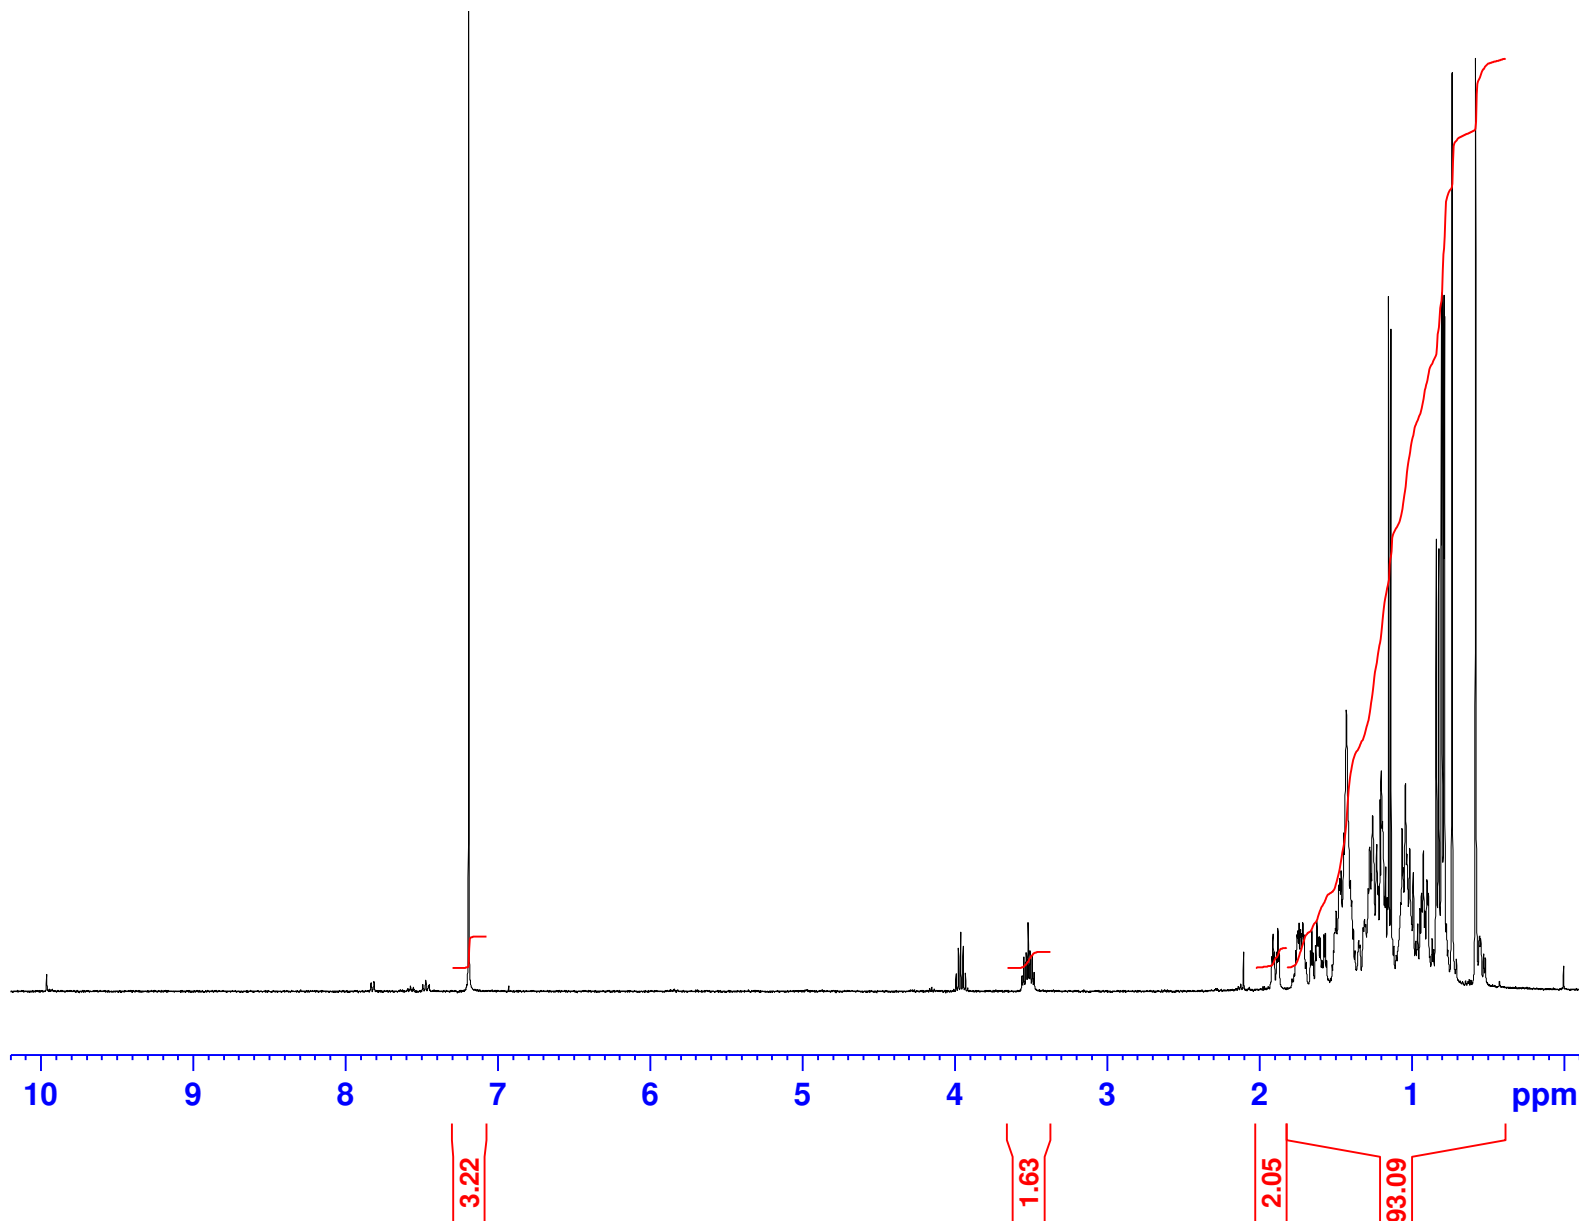

Current Data Parameters

NAME X_161116
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters

Date_ 20161116
Time 12.12
INSTRUM aviii400
PROBHD 5 mm PABBO BB-
PULPROG zg30
TD 65536
SOLVENT CDCl₃
NS 16
DS 0
SWH 8223.685 Hz
FIDRES 0.125483 Hz
AQ 3.9845889 sec
RG 228
DW 60.800 usec
DE 16.23 usec
TE 300.0 K
D1 1.00000000 sec
TD0 1

===== CHANNEL f1 =====

SFO1 400.2024714 MHz
NUC1 ¹H
P1 13.09 usec
PLW1 12.58899975 W

F2 - Processing parameters

SI 65536
SF 400.2000371 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00