


2016-12-13-130  
PROTON.qm CDCl3 /opt/data Adv\_Exp 23

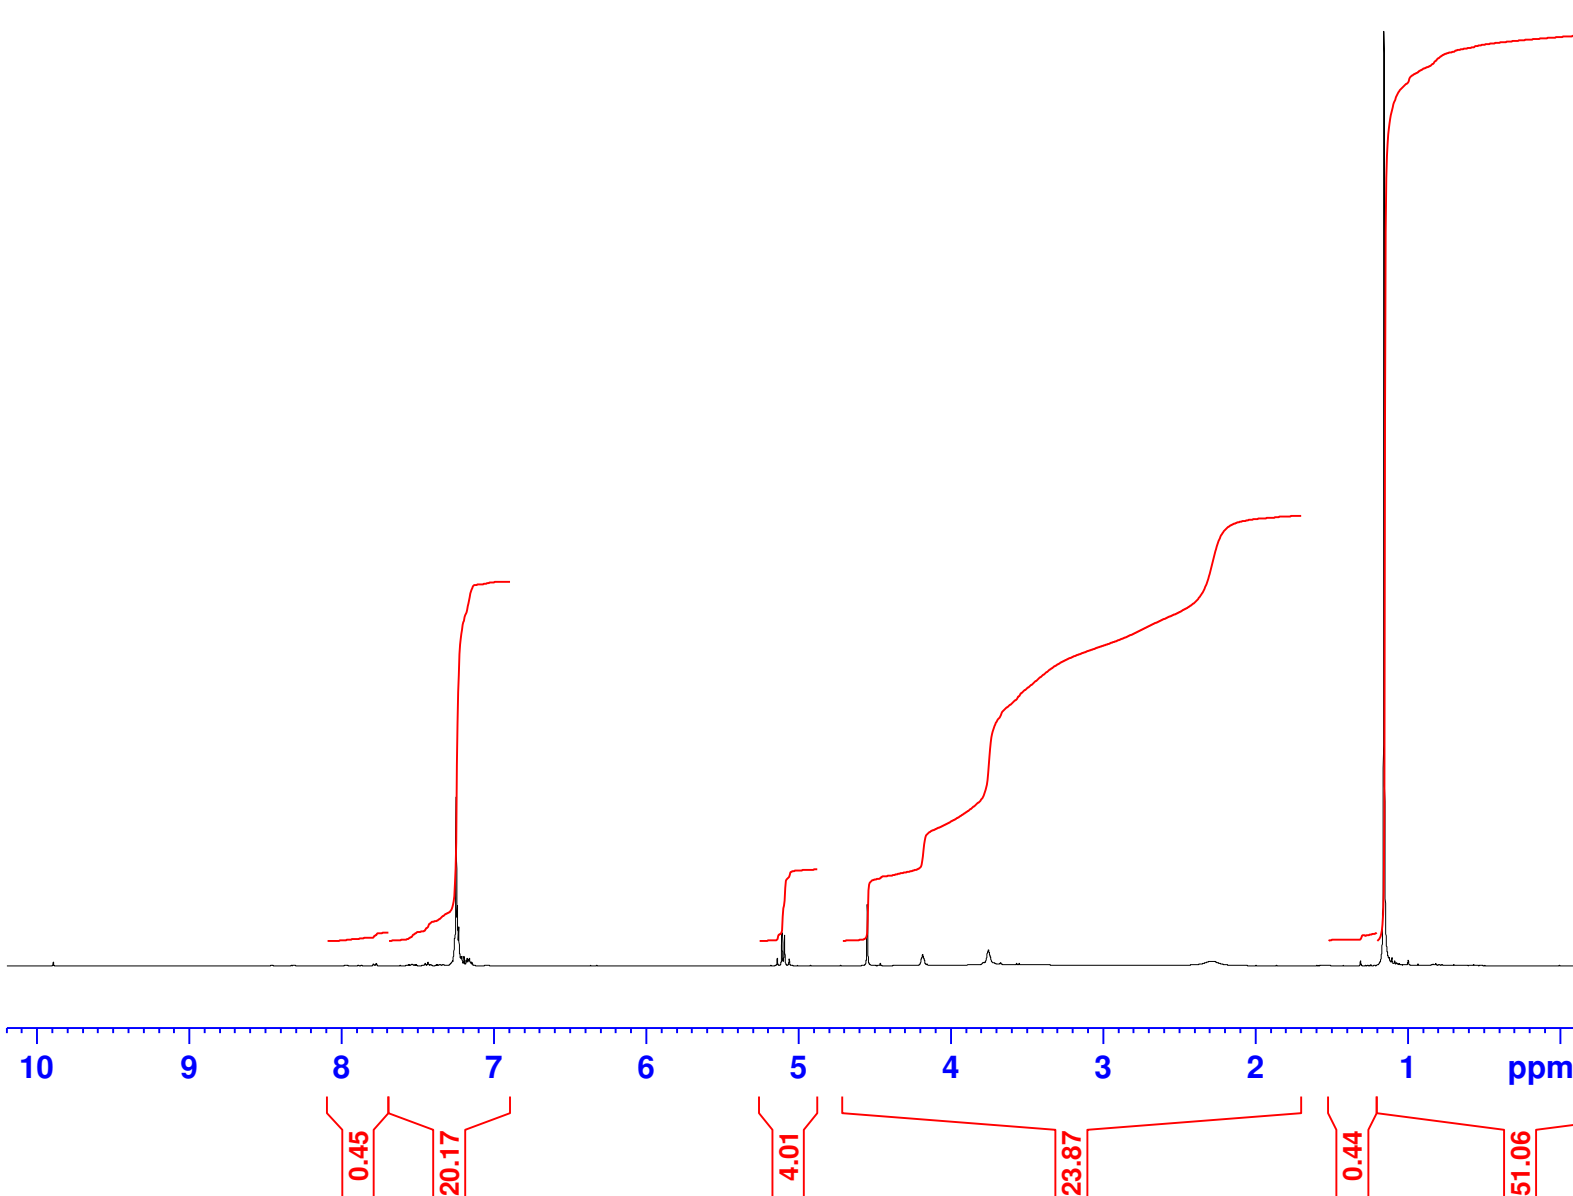

Current Data Parameters

NAME X\_161214  
EXPNO 130  
PROCNO 1

F2 - Acquisition Parameters

Date\_ 20161214  
Time 19.44  
INSTRUM aviii400  
PROBHD 5 mm PABBO BB-  
PULPROG zg30  
TD 65536  
SOLVENT CDCl3  
NS 16  
DS 0  
SWH 8223.685 Hz  
FIDRES 0.125483 Hz  
AQ 3.9845889 sec  
RG 25.4  
DW 60.800 usec  
DE 16.23 usec  
TE 300.0 K  
D1 1.00000000 sec  
TD0 1

===== CHANNEL f1 =====

SFO1 400.2024714 MHz  
NUC1 1H  
P1 13.09 usec  
PLW1 12.58899975 W

F2 - Processing parameters

SI 65536  
SF 400.2000350 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00