


Bilal Umarji - cat 1
P31CPD.qm CDC13 /opt/data Adv_Exp 10

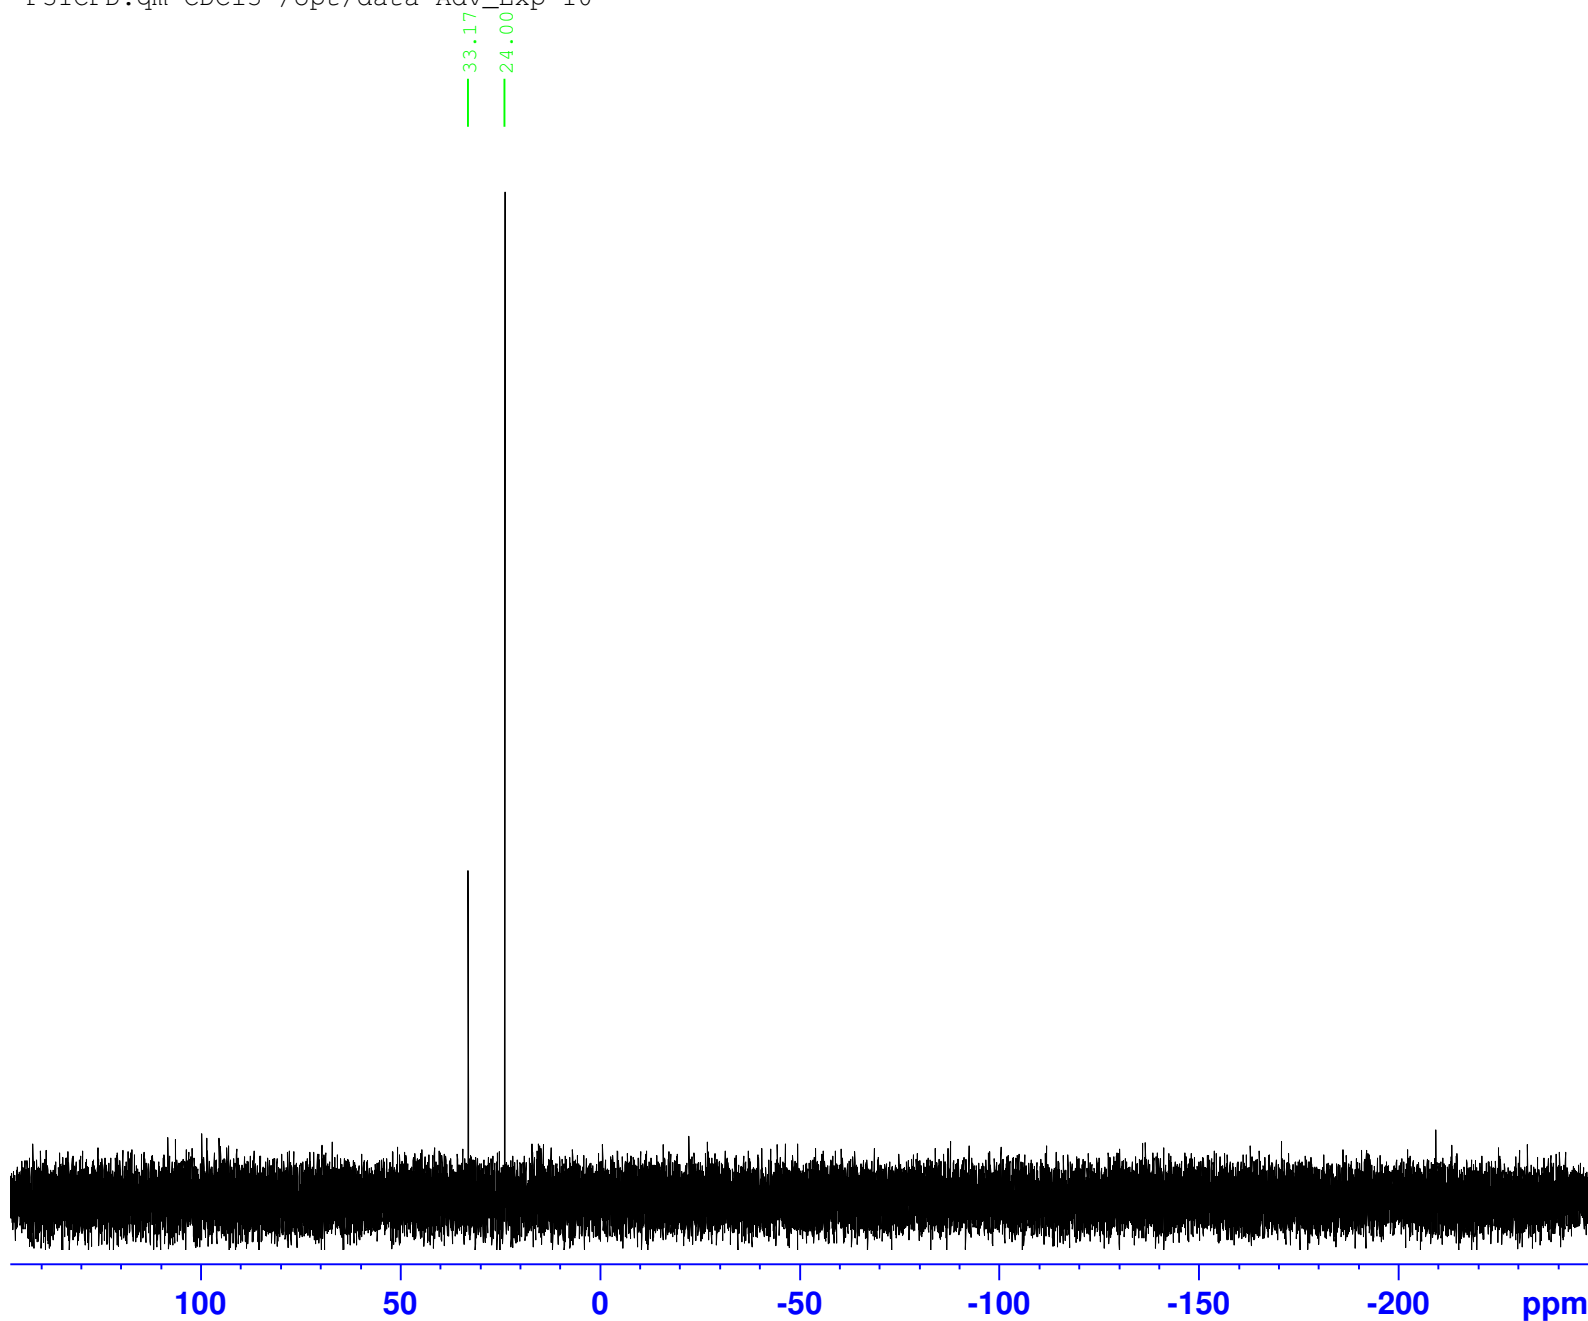

Current Data Parameters
NAME X_170111
EXPNO 222
PROCNO 1

F2 - Acquisition Parameters
Date_ 20170111
Time 12.41
INSTRUM aviii400
PROBHD 5 mm PABBO BB-
PULPROG zgig
TD 128198
SOLVENT CDC13
NS 32
DS 2
SWH 64102.562 Hz
FIDRES 0.500028 Hz
AQ 0.9999444 sec
RG 1620
DW 7.800 usec
DE 7.13 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 161.9958293 MHz
NUC1 31P
P1 11.30 usec
PLW1 19.05500031 W

===== CHANNEL f2 =====
SFO2 400.2024012 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 12.58899975 W
PLW12 0.26631001 W

F2 - Processing parameters
SI 262144
SF 162.0039290 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

1.95 0.13 0.33 0.92 0.40 1.46 1.13 0.30 3.54 1.10 0.93 6.40 1.98 1.87 1.36 0.71 1.09 0.98 0.59 0.02 1.29 1.22 0.48 0.42 0.74 1.02 0.93 1.58 0.00 0.99 0.81 1.41 0.52 0.28 0.52 1.02 0.23 0.71 0.20 0.76 0.79 0.90 0.52 0.11 2.47 0.22 1.01 0.91 0.98