

AS Pure
P31CPD.qm CDC13 /opt/data Adv_Exp 5


Current Data Parameters
NAME X_170222
EXPNO 162
PROCNO 1

F2 - Acquisition Parameters
Date_ 20170222
Time 15.06
INSTRUM aviii400
PROBHD 5 mm PABBO BB-
PULPROG zgig
TD 128198
SOLVENT CDC13
NS 32
DS 2
SWH 64102.562 Hz
FIDRES 0.500028 Hz
AQ 0.9999444 sec
RG 1620
DW 7.800 usec
DE 7.13 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 161.9958293 MHz
NUC1 31P
P1 11.30 usec
PLW1 19.05500031 W

===== CHANNEL f2 =====
SFO2 400.2024012 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 12.58899975 W
PLW12 0.26631001 W

F2 - Processing parameters
SI 262144
SF 162.0039290 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

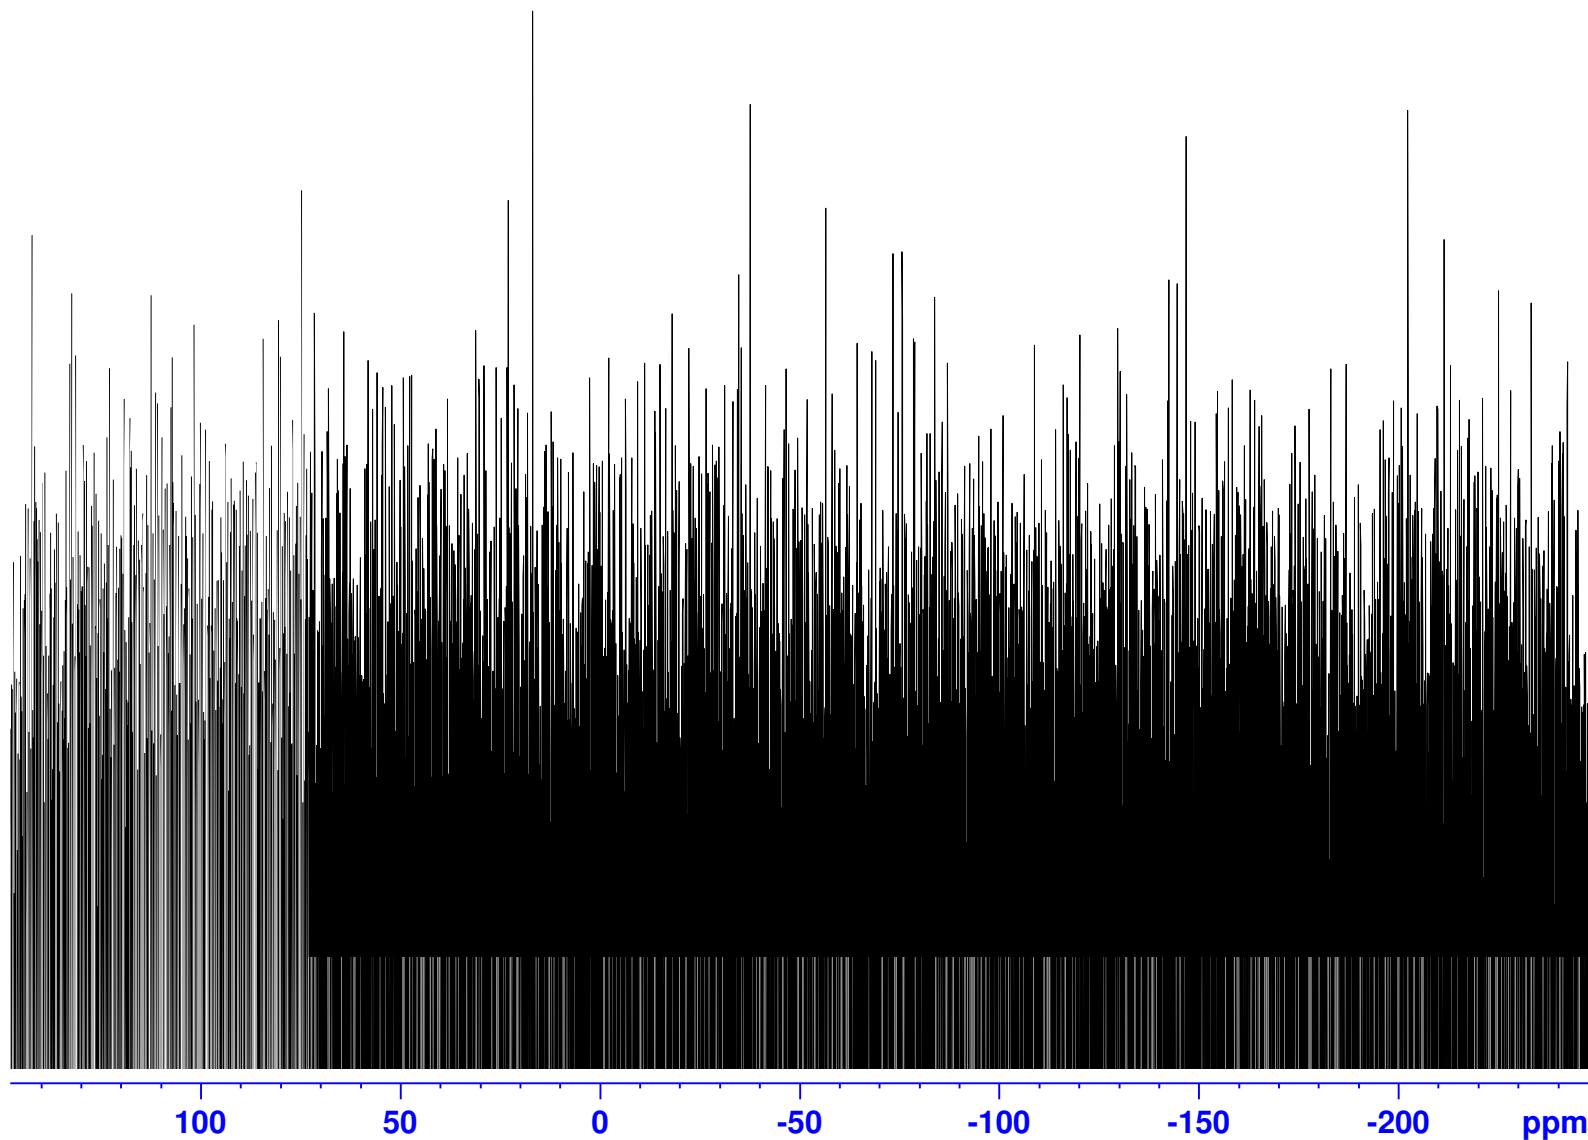

1.00 1.27 1.28 1.20 0.02 2.05 0.53 0.43 1.71 1.23 2.64 0.50 1.12 1.09 0.10 0.82 0.23 1.63 0.29 0.74 1.09 0.77 0.28 1.24 0.81 0.34 0.38 1.43 0.86 1.22 1.55 0.68 0.84 0.79 1.39 1.47 1.96 1.19 2.13 1.45 1.15 2.38 1.90 1.36 1.79 0.64 1.33 0.97