


pure A
P31CPD.qm CDC13 /opt/data Adv_Exp 9

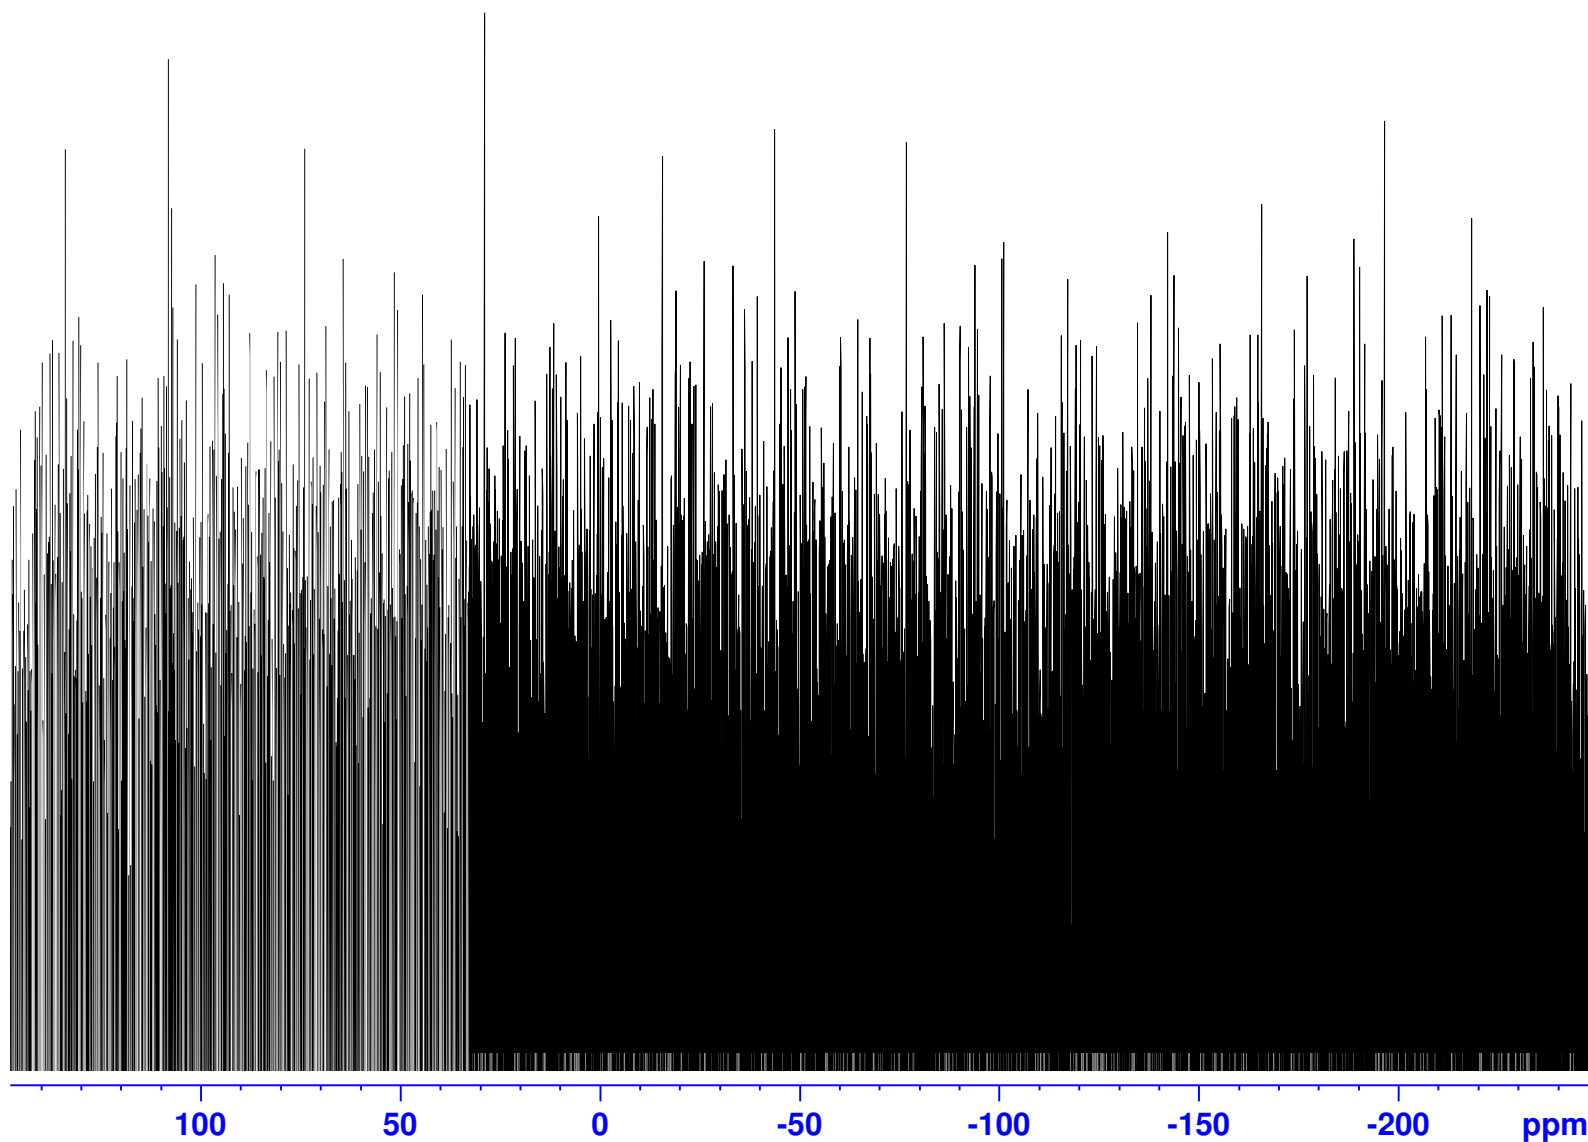

Current Data Parameters
NAME X_170223
EXPNO 71
PROCNO 1

F2 - Acquisition Parameters
Date_ 20170223
Time 15.34
INSTRUM aviii400
PROBHD 5 mm PABBO BB-
PULPROG zgig
TD 128198
SOLVENT CDC13
NS 32
DS 2
SWH 64102.562 Hz
FIDRES 0.500028 Hz
AQ 0.9999444 sec
RG 1620
DW 7.800 usec
DE 7.13 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 161.9958293 MHz
NUC1 31P
P1 11.30 usec
PLW1 19.05500031 W

===== CHANNEL f2 =====
SFO2 400.2024012 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 12.58899975 W
PLW12 0.26631001 W

F2 - Processing parameters
SI 262144
SF 162.0039290 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

0.62 0.54 1.59 0.73 1.25 1.04 0.34 0.70 1.03 1.45 2.67 0.04 1.51 0.82 0.99 2.40 1.28 2.06 1.02 0.78 0.31 0.34 0.84 0.30 1.09 0.48 1.12 0.49 0.46 0.69 1.78 1.21 0.96 0.68 2.26 0.61 0.86 2.62 1.73 0.28 0.75 0.19 0.52 0.91 2.02 2.41 2.92 1.79 0.48