


Current Data Parameters
NAME X_170920
EXPNO 152
PROCNO 1

F2 - Acquisition Parameters
Date_ 20170920
Time 19.05 h
INSTRUM aviii400
PROBHD Z108618_0305 (
PULPROG zgig
TD 128198
SOLVENT CDC13
NS 32
DS 2
SWH 64102.562 Hz
FIDRES 1.000056 Hz
AQ 0.9999444 sec
RG 2050
DW 7.800 usec
DE 7.13 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 161.9958293 MHz
NUC1 31P
P1 11.30 usec
PLW1 19.05500031 W
SFO2 400.2024012 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 12.58899975 W
PLW12 0.26631001 W

F2 - Processing parameters
SI 262144
SF 162.0039290 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

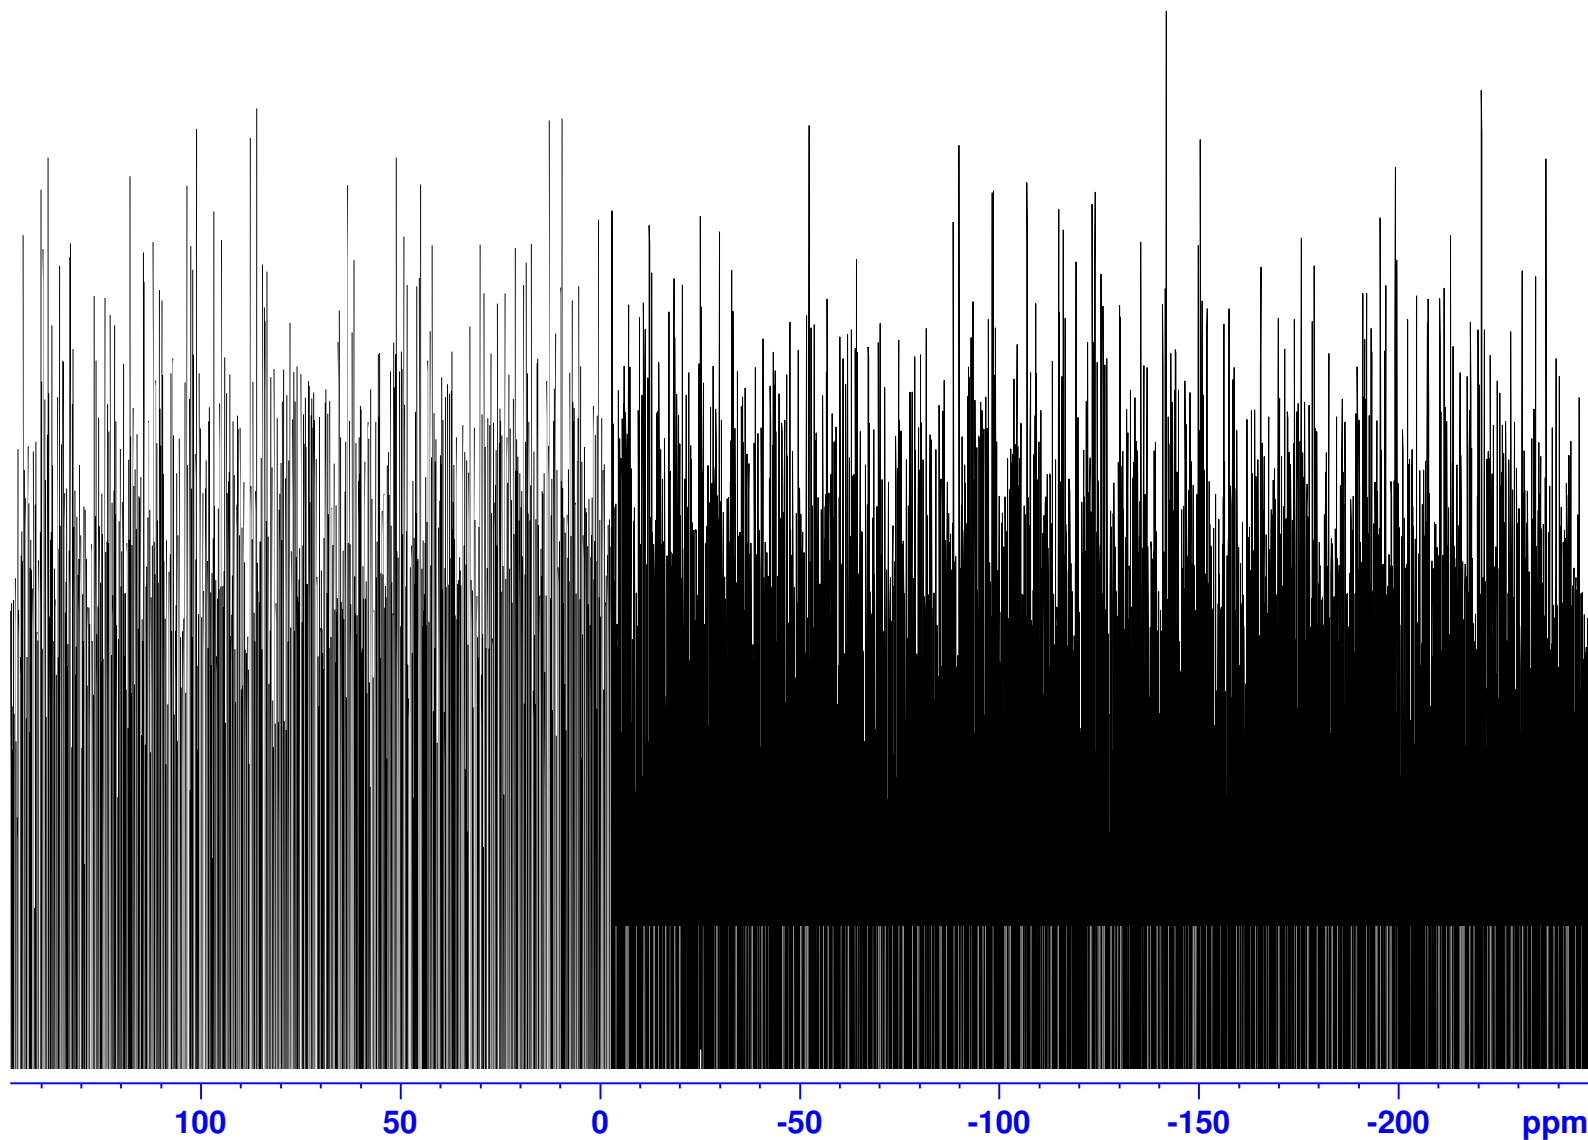

3.13 0.99 0.40 1.49 0.60 0.45 0.70 1.39 2.01 1.42 1.81 1.75 0.65 0.51 3.20 2.42 1.29 3.14 0.19 1.68 0.22 2.39 1.29 0.69 0.97 0.51 1.92 1.40 1.30 0.16 0.22 0.87 0.03 0.15 0.08 0.33 1.92 1.06 0.68 1.93 1.20 1.27 2.00 0.45 1.48 0.86 0.63 1.58 1.57