


PdCl<sub>2</sub>PPh<sub>3</sub> MM  
PROTON.qm CDCl<sub>3</sub> /opt/data Adv\_Exp 50

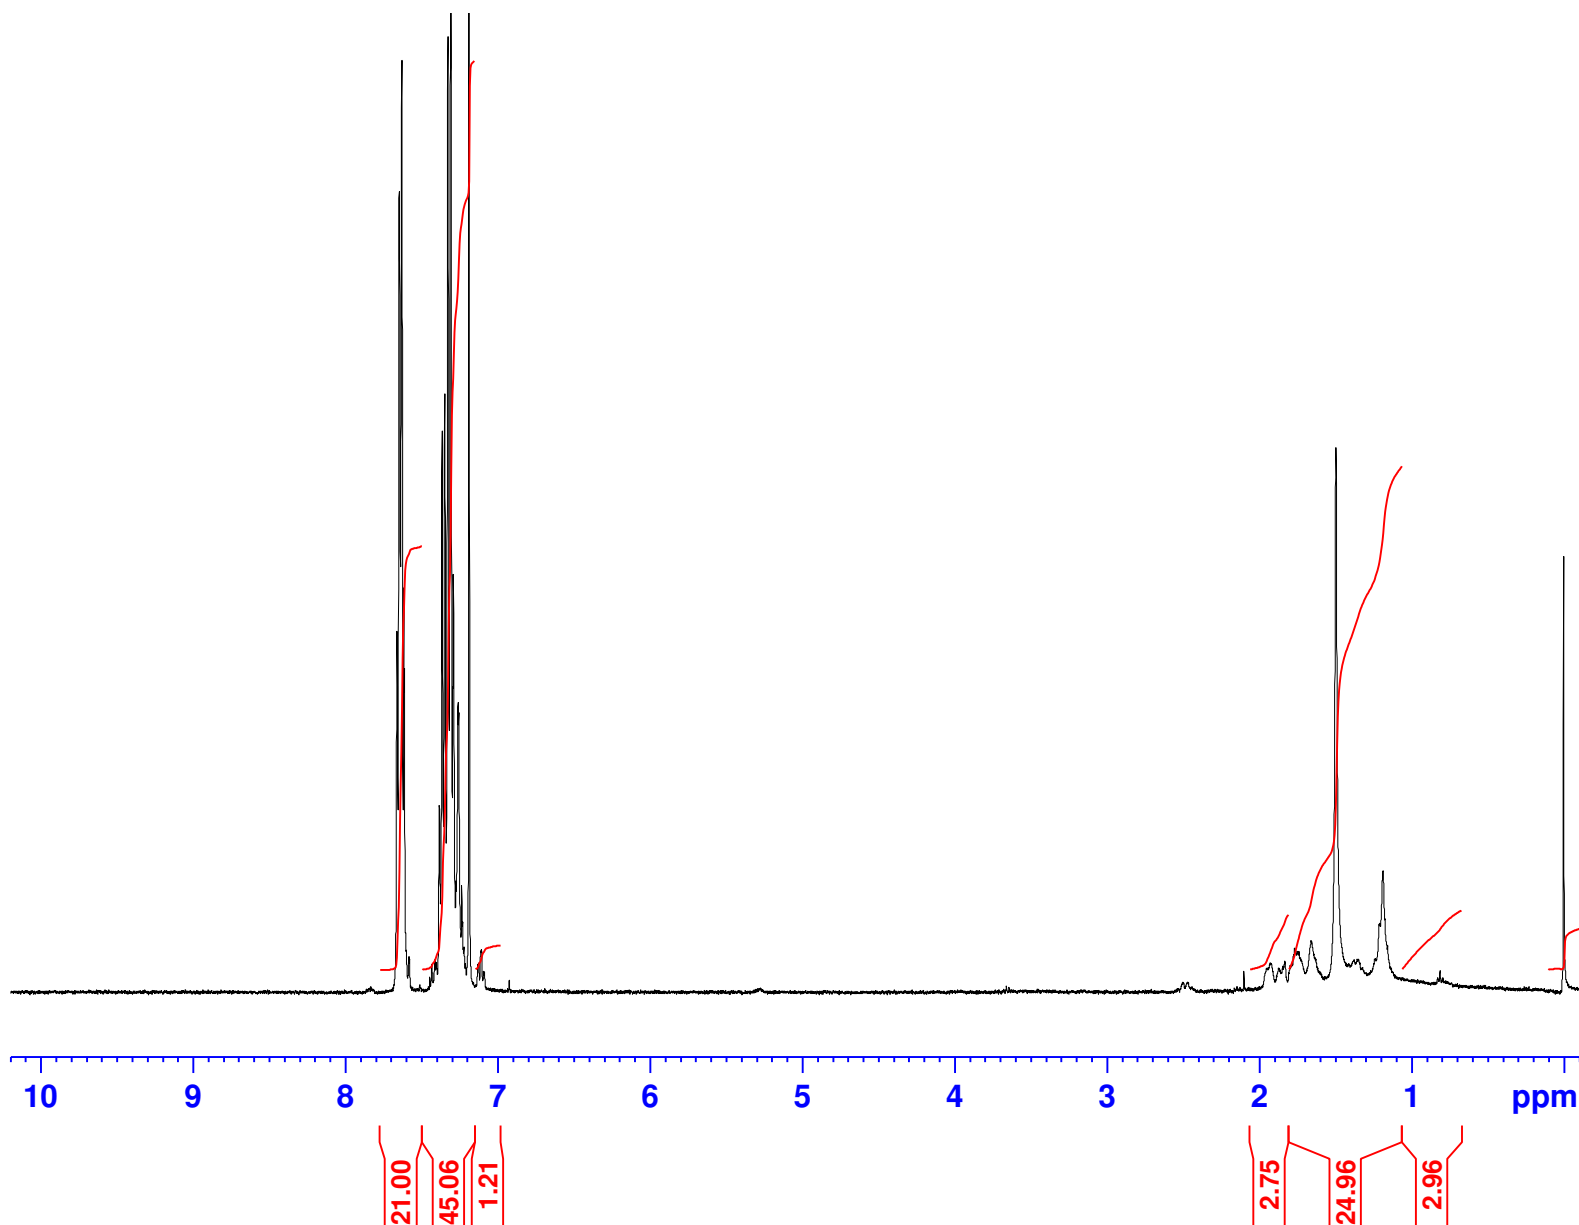

Current Data Parameters  
NAME X\_171107  
EXPNO 90  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20171108  
Time 0.49 h  
INSTRUM aviii400  
PROBHD Z108618\_0305 (  
PULPROG zg30  
TD 65536  
SOLVENT CDCl<sub>3</sub>  
NS 16  
DS 0  
SWH 8223.685 Hz  
FIDRES 0.250967 Hz  
AQ 3.9845889 sec  
RG 406  
DW 60.800 usec  
DE 16.23 usec  
TE 300.0 K  
D1 1.00000000 sec  
TD0 1  
SFO1 400.2024714 MHz  
NUC1 1H  
P1 13.09 usec  
PLW1 12.58899975 W

F2 - Processing parameters  
SI 65536  
SF 400.2000383 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00