


palmo product 2  
P31CPD.qm CDC13 /opt/data Adv\_Exp 13

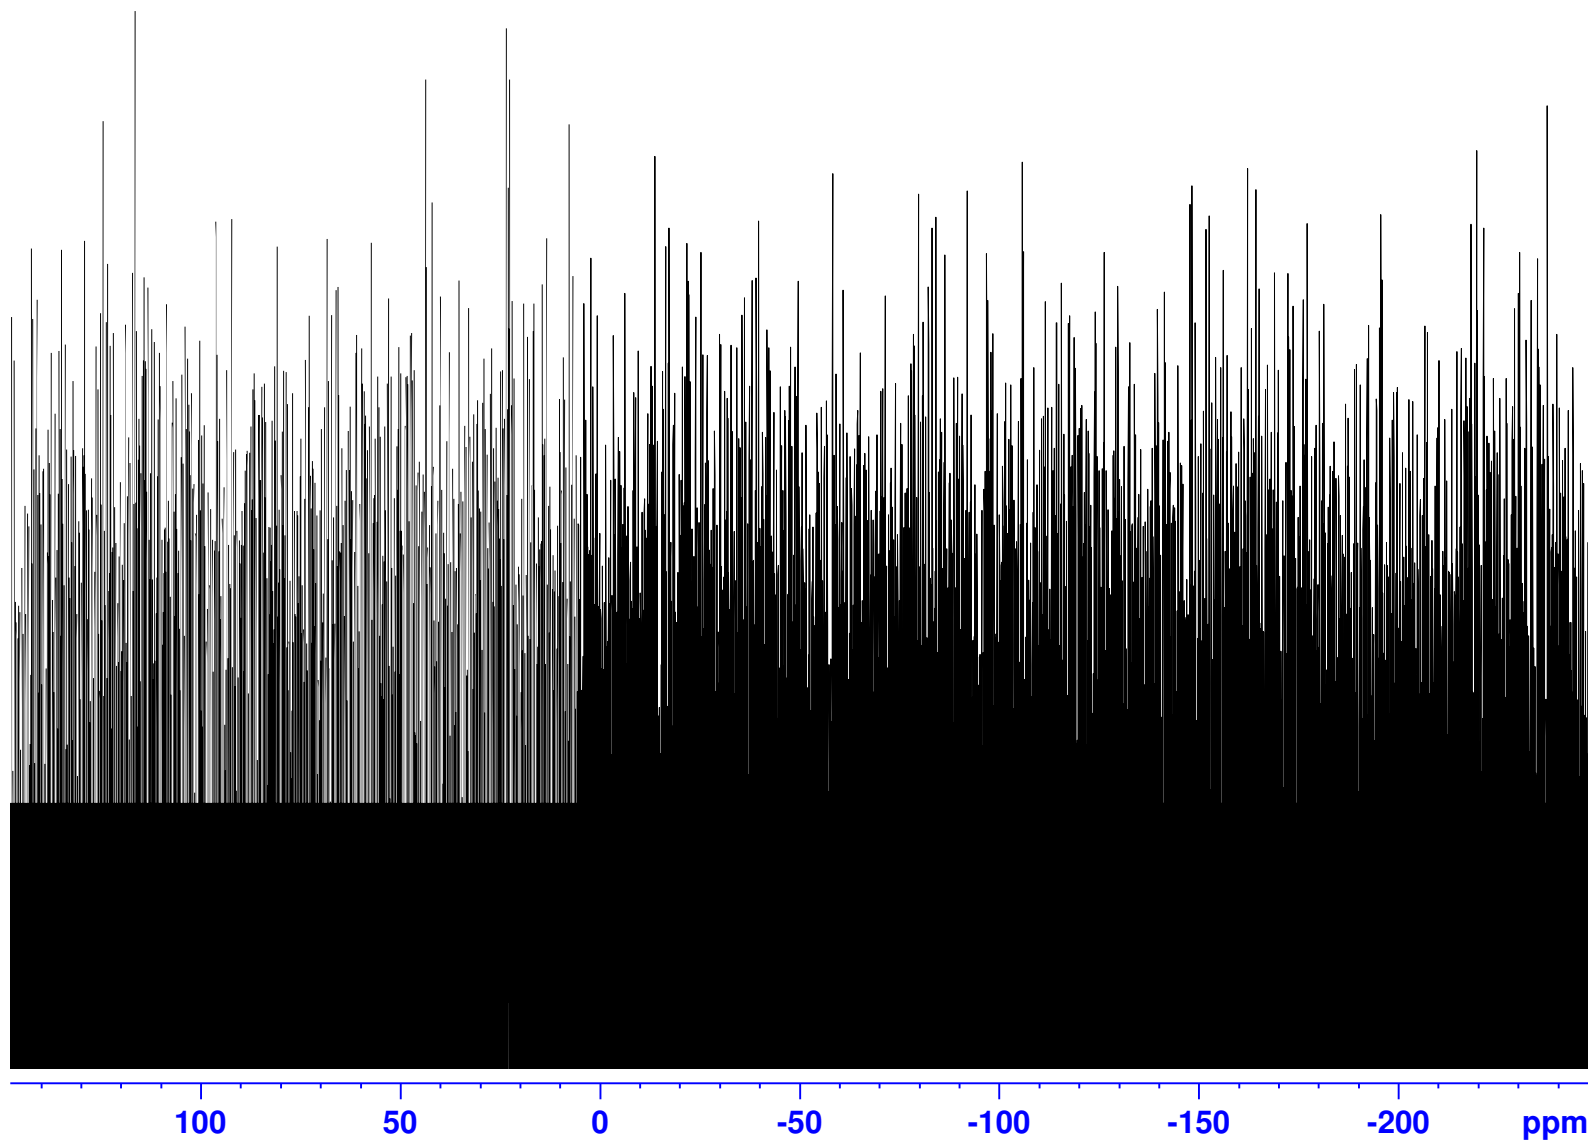

Current Data Parameters  
NAME X\_171108  
EXPNO 112  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20171109  
Time 0.44 h  
INSTRUM aviii400  
PROBHD Z108618\_0305 (  
PULPROG zgig  
TD 128198  
SOLVENT CDC13  
NS 32  
DS 2  
SWH 64102.562 Hz  
FIDRES 1.000056 Hz  
AQ 0.9999444 sec  
RG 1620  
DW 7.800 usec  
DE 7.13 usec  
TE 300.0 K  
D1 2.00000000 sec  
D11 0.03000000 sec  
TD0 1  
SFO1 161.9958293 MHz  
NUC1 31P  
P1 11.30 usec  
PLW1 19.05500031 W  
SFO2 400.2024012 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 12.58899975 W  
PLW12 0.26631001 W

F2 - Processing parameters  
SI 262144  
SF 162.0039290 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40

1.06 1.68 3.31 2.04 1.83 0.16 0.58 1.74 0.71 1.85 0.62 7.62 0.68 1.06 0.34 0.74 1.51 1.02 0.17 1.34 1.45 0.71 0.63 0.59 0.47 0.81 1.27 1.75 1.20 2.00 0.79 0.40 1.64 1.42 1.98 1.14 0.40 1.15 1.70 2.19 1.28 0.96 0.60 1.38 0.04 0.22 0.17 1.20 0.56