


aditya cat 1
P31CPD.qm CDC13 /opt/data Adv_Exp 32

Current Data Parameters
NAME X_180221
EXPNO 42
PROCNO 1

F2 - Acquisition Parameters
Date_ 20180221
Time 15.39 h
INSTRUM aviii400
PROBHD Z108618_0305 (
PULPROG zgig
TD 128198
SOLVENT CDC13
NS 32
DS 2
SWH 64102.562 Hz
FIDRES 1.000056 Hz
AQ 0.9999444 sec
RG 1620
DW 7.800 usec
DE 7.13 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 161.9958293 MHz
NUC1 31P
P1 11.30 usec
PLW1 19.05500031 W
SFO2 400.2024012 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 12.58899975 W
PLW12 0.26631001 W

F2 - Processing parameters
SI 262144
SF 162.0039290 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

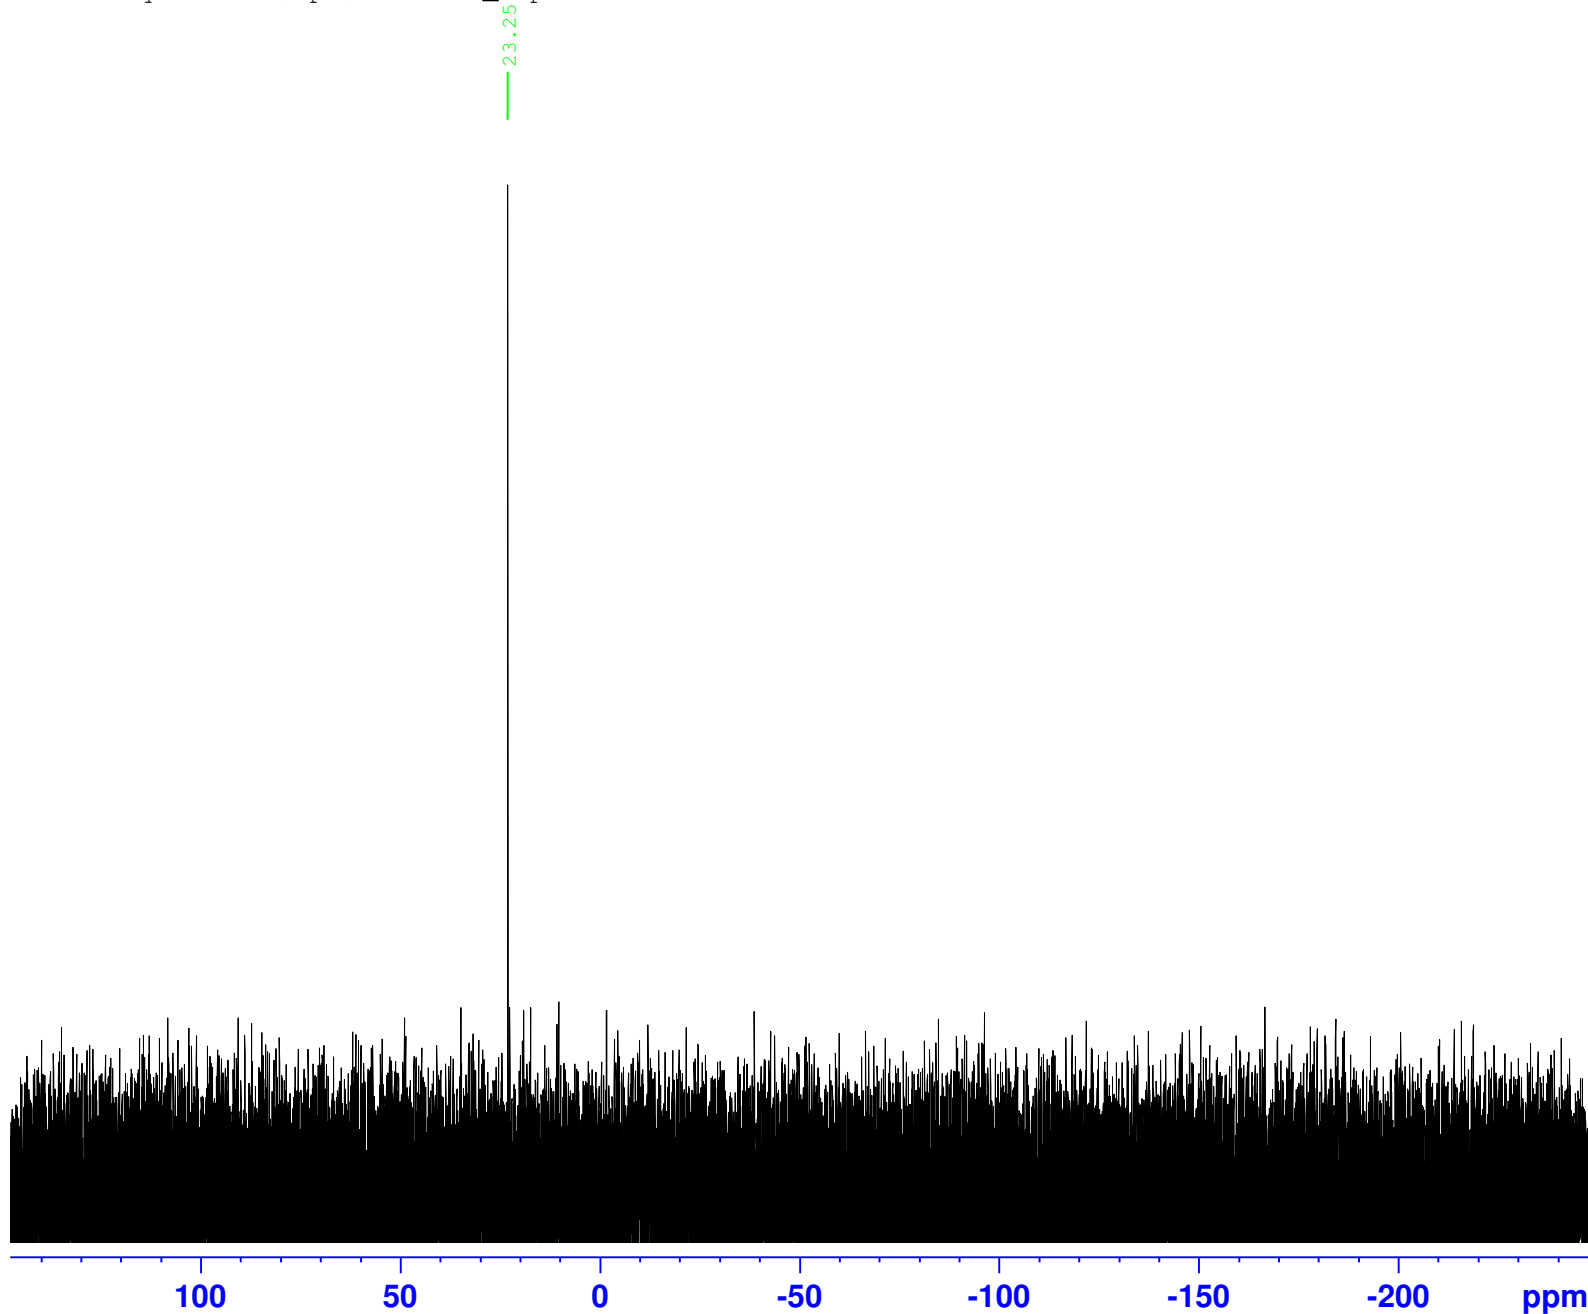

1.12 0.74 0.64 0.15 2.39 1.80 0.92 1.38 0.28 5.53 0.62 1.75 2.96 0.64 1.17 0.67 4.12 1.20 1.89 1.15 0.11 0.14 2.61 1.18 0.32 0.67 0.21 1.23 0.45 1.40 1.75 0.26 0.37 1.76 1.10 1.27 0.48 0.01 2.04 1.45 1.79 0.92 0.22 0.76 2.04 0.71 0.25 0.98 1.19