


aditya 1 pure product  
P31CPD.qm CDC13 /opt/data Adv\_Exp 31

34.16  
31.75

Current Data Parameters  
NAME X\_180222  
EXPNO 12  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20180222  
Time 13.43 h  
INSTRUM aviii400  
PROBHD Z108618\_0305 (  
PULPROG zgig  
TD 128198  
SOLVENT CDC13  
NS 32  
DS 2  
SWH 64102.562 Hz  
FIDRES 1.000056 Hz  
AQ 0.9999444 sec  
RG 1620  
DW 7.800 usec  
DE 7.13 usec  
TE 300.0 K  
D1 2.00000000 sec  
D11 0.03000000 sec  
TD0 1  
SFO1 161.9958293 MHz  
NUC1 31P  
P1 11.30 usec  
PLW1 19.05500031 W  
SFO2 400.2024012 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 12.58899975 W  
PLW12 0.26631001 W

F2 - Processing parameters  
SI 262144  
SF 162.0039290 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40

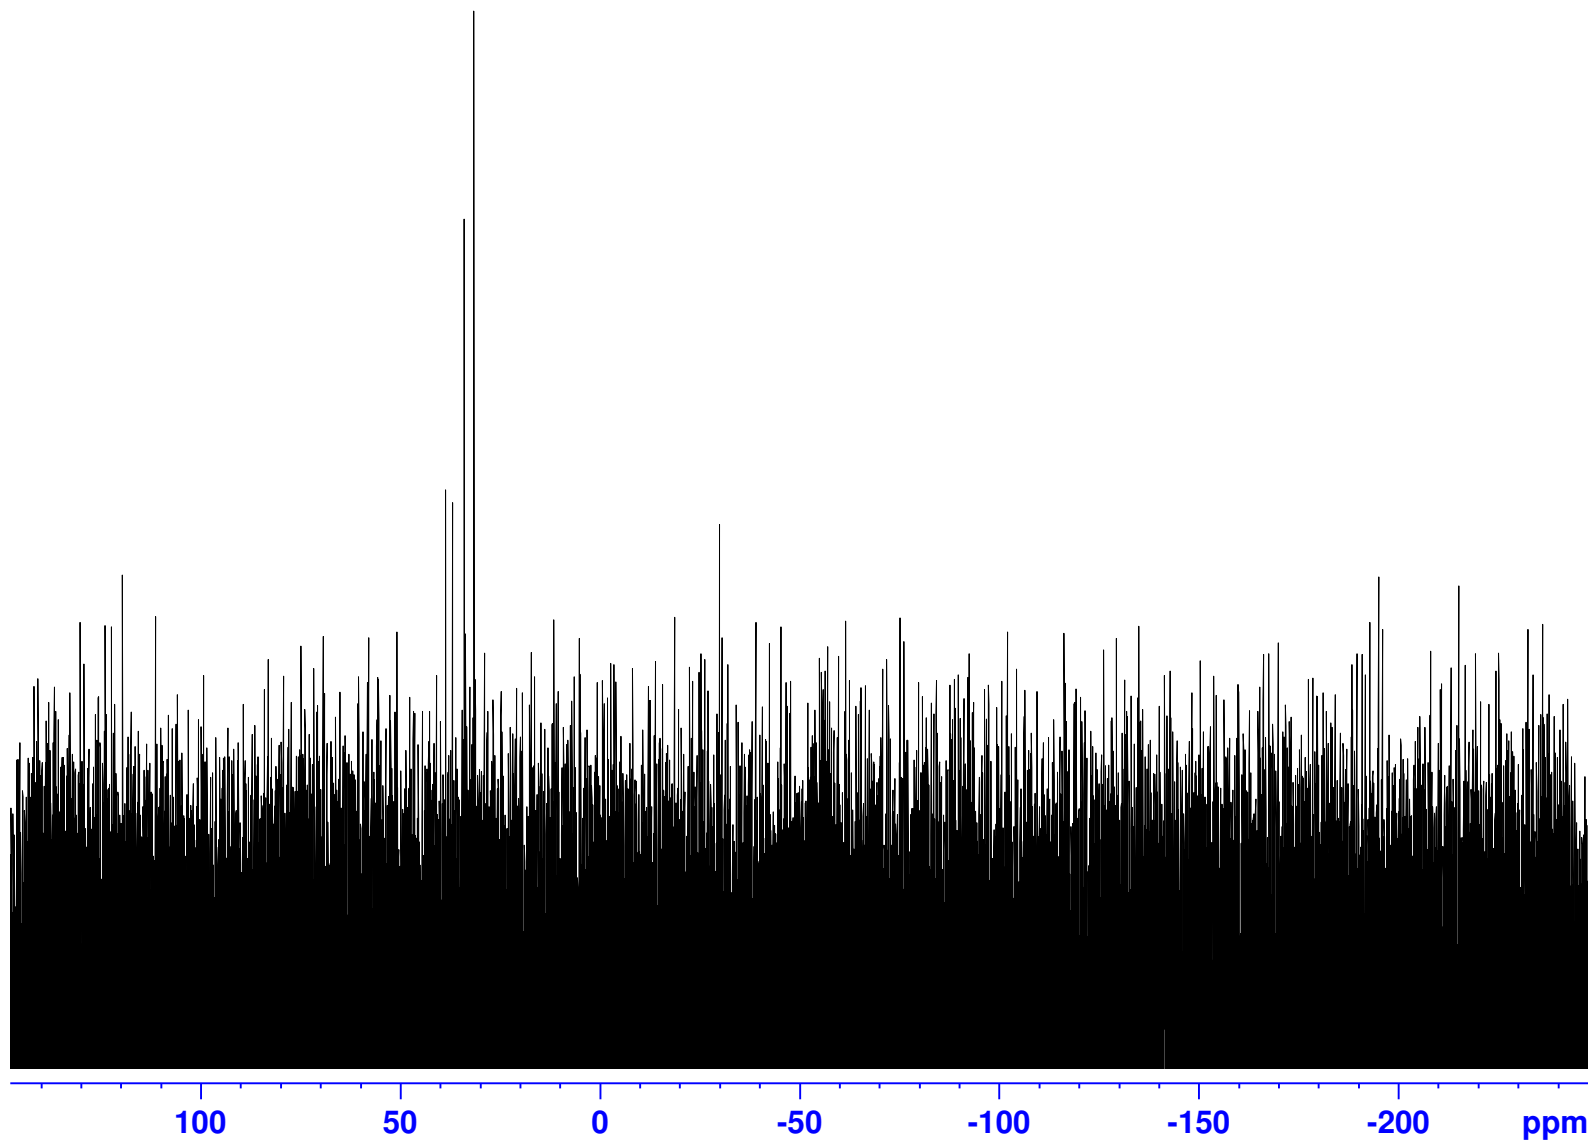

0.73  
0.30  
1.46  
4.78  
0.36  
1.72  
1.72  
1.59  
0.60  
0.86  
2.54  
0.75  
0.63  
0.07  
0.34  
1.95  
0.91  
1.04  
0.86  
2.33  
0.88  
2.00  
0.20  
2.21  
0.80  
1.30  
1.57  
0.95  
0.72  
1.48  
2.01  
0.12  
1.03  
2.43  
0.19  
0.95  
0.19  
1.76  
1.22  
0.19  
3.55  
0.27  
1.72  
0.56  
1.21  
2.58  
0.60  
0.83  
1.72