


Current Data Parameters
NAME X_180222
EXPNO 62
PROCNO 1

F2 - Acquisition Parameters
Date_ 20180223
Time 18.28 h
INSTRUM aviii400
PROBHD Z108618_0305 (
PULPROG zgig
TD 128198
SOLVENT CDC13
NS 32
DS 2
SWH 64102.562 Hz
FIDRES 1.000056 Hz
AQ 0.9999444 sec
RG 2050
DW 7.800 usec
DE 7.13 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 161.9958293 MHz
NUC1 31P
P1 11.30 usec
PLW1 19.05500031 W
SFO2 400.2024012 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 12.58899975 W
PLW12 0.26631001 W

F2 - Processing parameters
SI 262144
SF 162.0039290 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

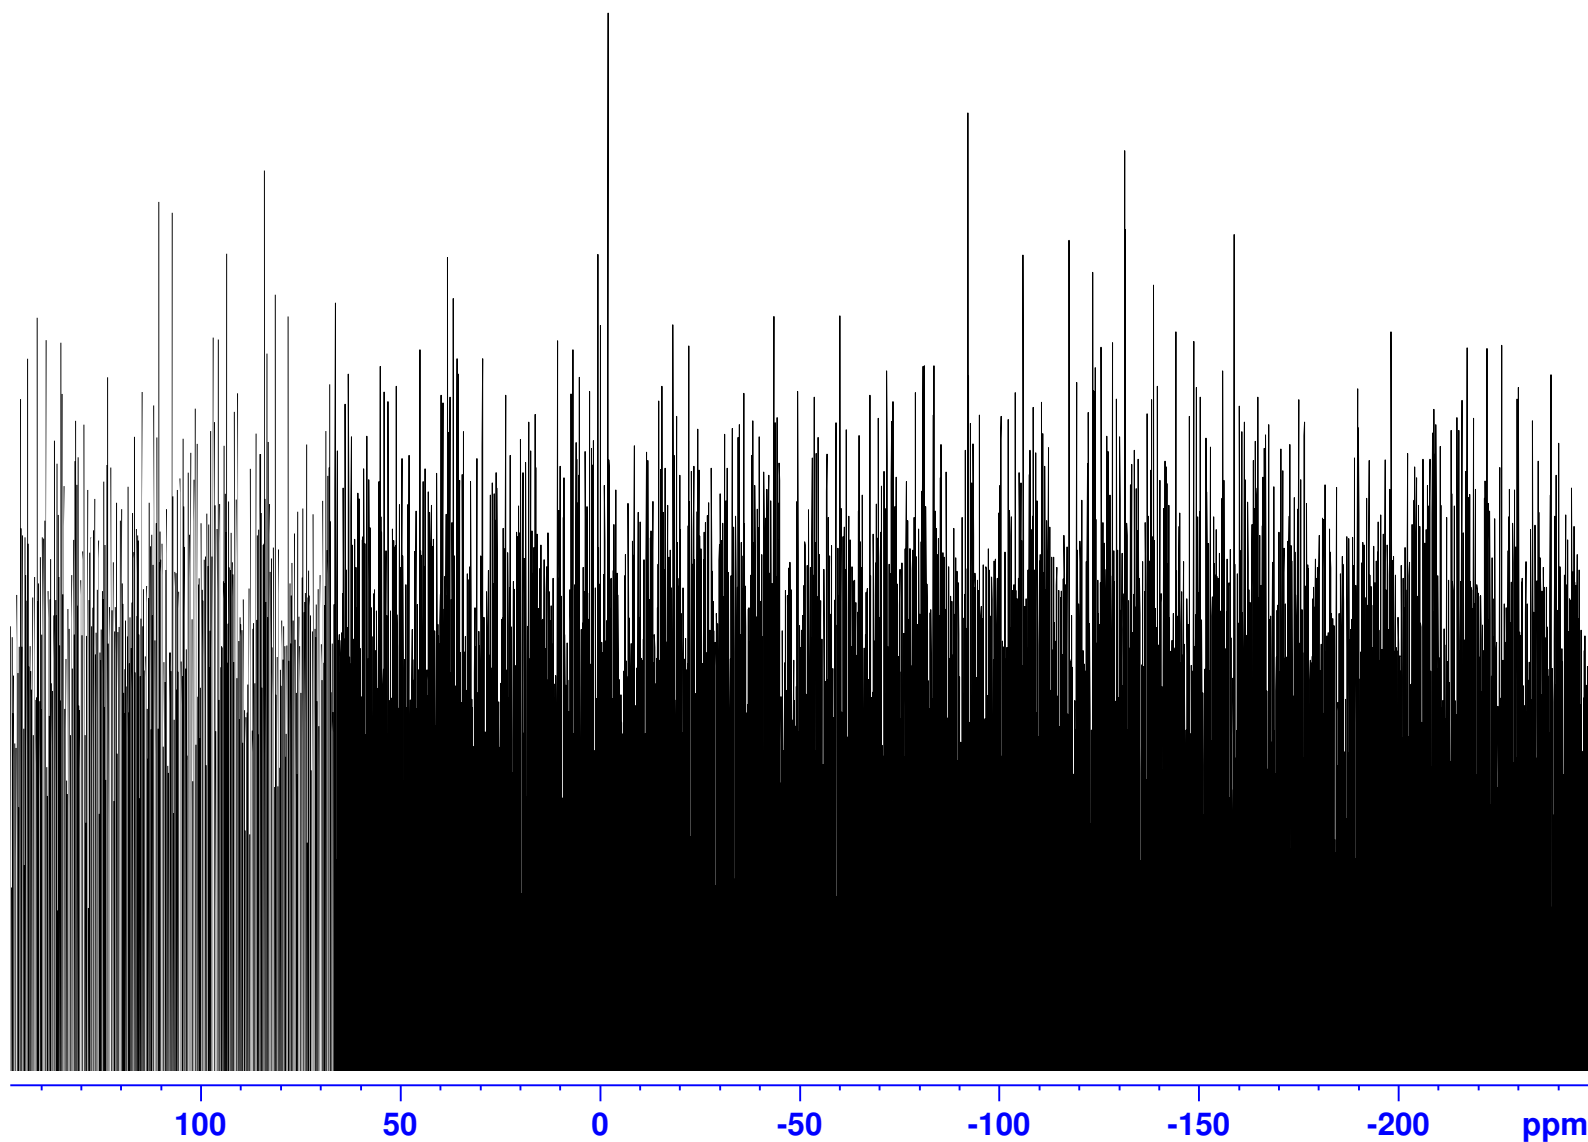

1.48 0.70 0.41 2.21 1.60 1.84 1.96 1.40 1.33 1.56 3.33 2.70 1.29 0.89 0.17 1.36 2.17 0.24 0.68 0.14 2.58 0.91 0.26 1.56 1.02 0.56 1.31 1.63 1.51 1.66 1.09 2.04 0.61 0.27 0.61 0.44 0.98 1.15 0.21 2.11 0.24 0.99 2.33 0.61 0.43 2.55 1.29 0.26