


suad\_cr\_a

P31CPD.qm CDC13 /opt/data Adv\_Exp 5

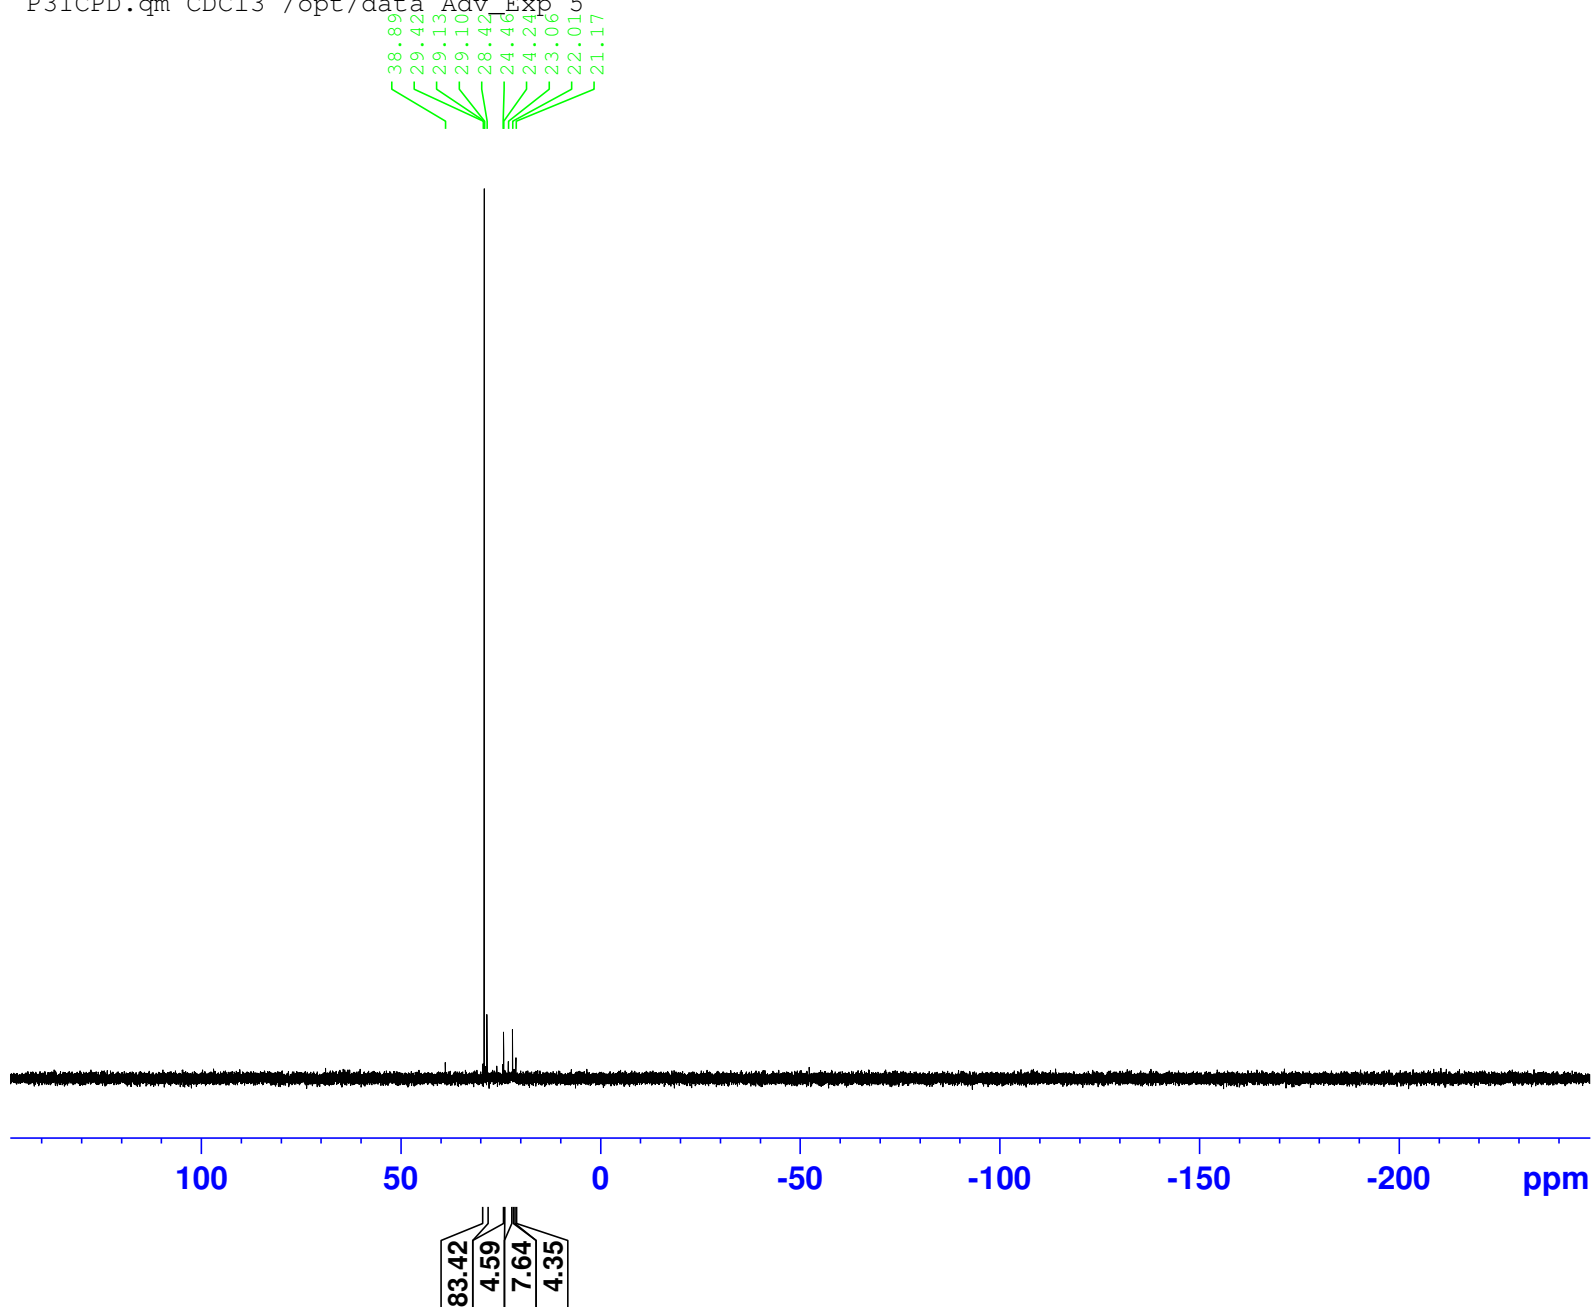

#### Current Data Parameters

NAME X\_180920  
EXPNO 82  
PROCNO 1

#### F2 - Acquisition Parameters

Date\_ 20180920  
Time 21.12 h  
INSTRUM aviii400  
PROBHD z108618\_0305 (   
PULPROG zgig  
TD 128198  
SOLVENT CDC13  
NS 32  
DS 2  
SWH 64102.562 Hz  
FIDRES 1.000056 Hz  
AQ 0.9999444 sec  
RG 1620  
DW 7.800 usec  
DE 7.13 usec  
TE 300.0 K  
D1 2.00000000 sec  
D11 0.03000000 sec  
TD0 1  
SFO1 161.9958293 MHz  
NUC1 31P  
P1 11.30 usec  
PLW1 19.05500031 W  
SFO2 400.2024012 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 19.95299911 W  
PLW12 0.36664000 W

#### F2 - Processing parameters

SI 262144  
SF 162.0039290 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40