


maz ahmed pdc12(pph3)2
P31CPD CDCl3 /opt/data Adv_Exp 12

25.00

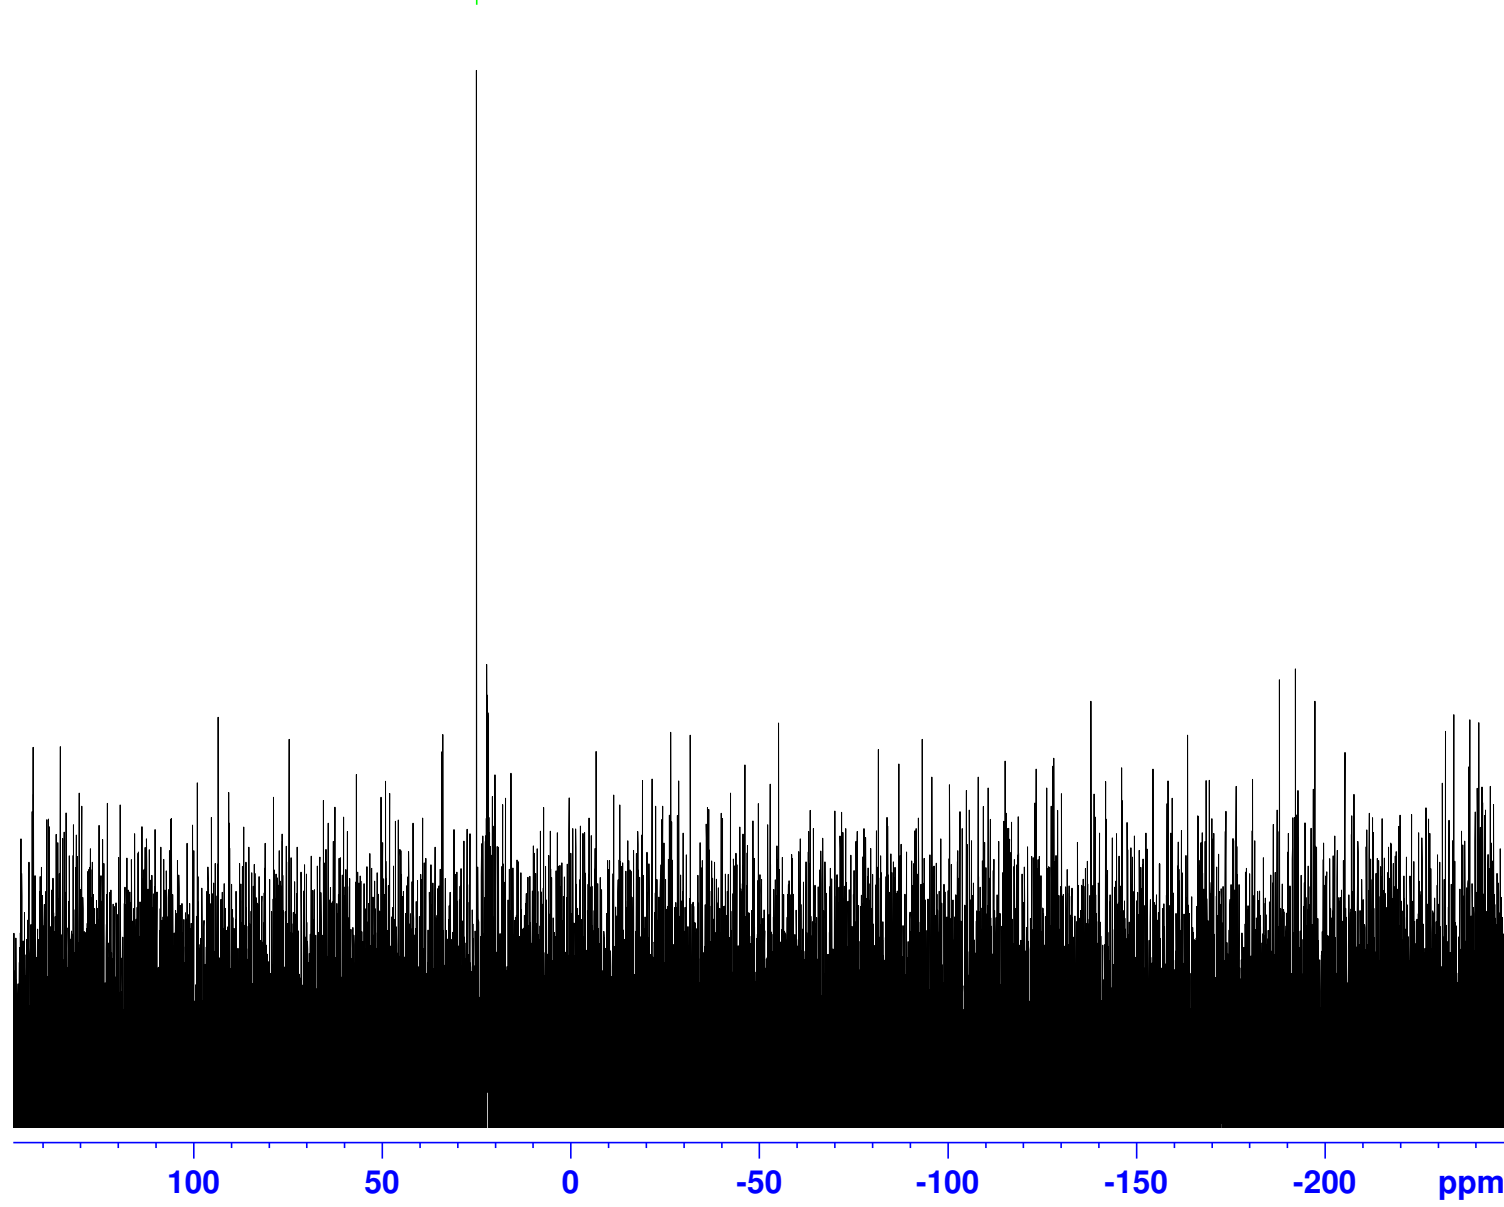

Current Data Parameters
NAME X_20180918
EXPNO 62
PROCNO 1

F2 - Acquisition Parameters
Date_ 20180918
Time 13.32 h
INSTRUM spect
PROBHD Z824801_0046 (
PULPROG zgpg30
TD 65536
SOLVENT CDCl3
NS 16
DS 4
SWH 64102.562 Hz
FIDRES 1.956255 Hz
AQ 0.5111808 sec
RG 200.25
DW 7.800 usec
DE 6.50 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 162.0079729 MHz
NUC1 31P
P0 2.67 usec
P1 8.00 usec
PLW1 36.45100021 W
SFO2 400.2316009 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.23714000 W
PLW13 0.11928000 W

F2 - Processing parameters
SI 32768
SF 162.0160737 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

1.05 0.21 0.11 0.94 1.35 1.34 0.59 1.65 9.77 2.48 0.24 0.21 1.32 0.18 0.34 0.57 0.48 0.84 1.04 1.13 0.73 1.67 0.13 1.46 0.25 1.01 0.66 0.51 0.96 0.41 0.07 1.01 0.88 0.90 0.61 1.66 0.45 1.50 0.90 1.15 0.16 1.35 0.16 0.74 0.80 1.29