


vb part 2 final pure
P31CPD CDC13 /opt/data Adv_Exp 4

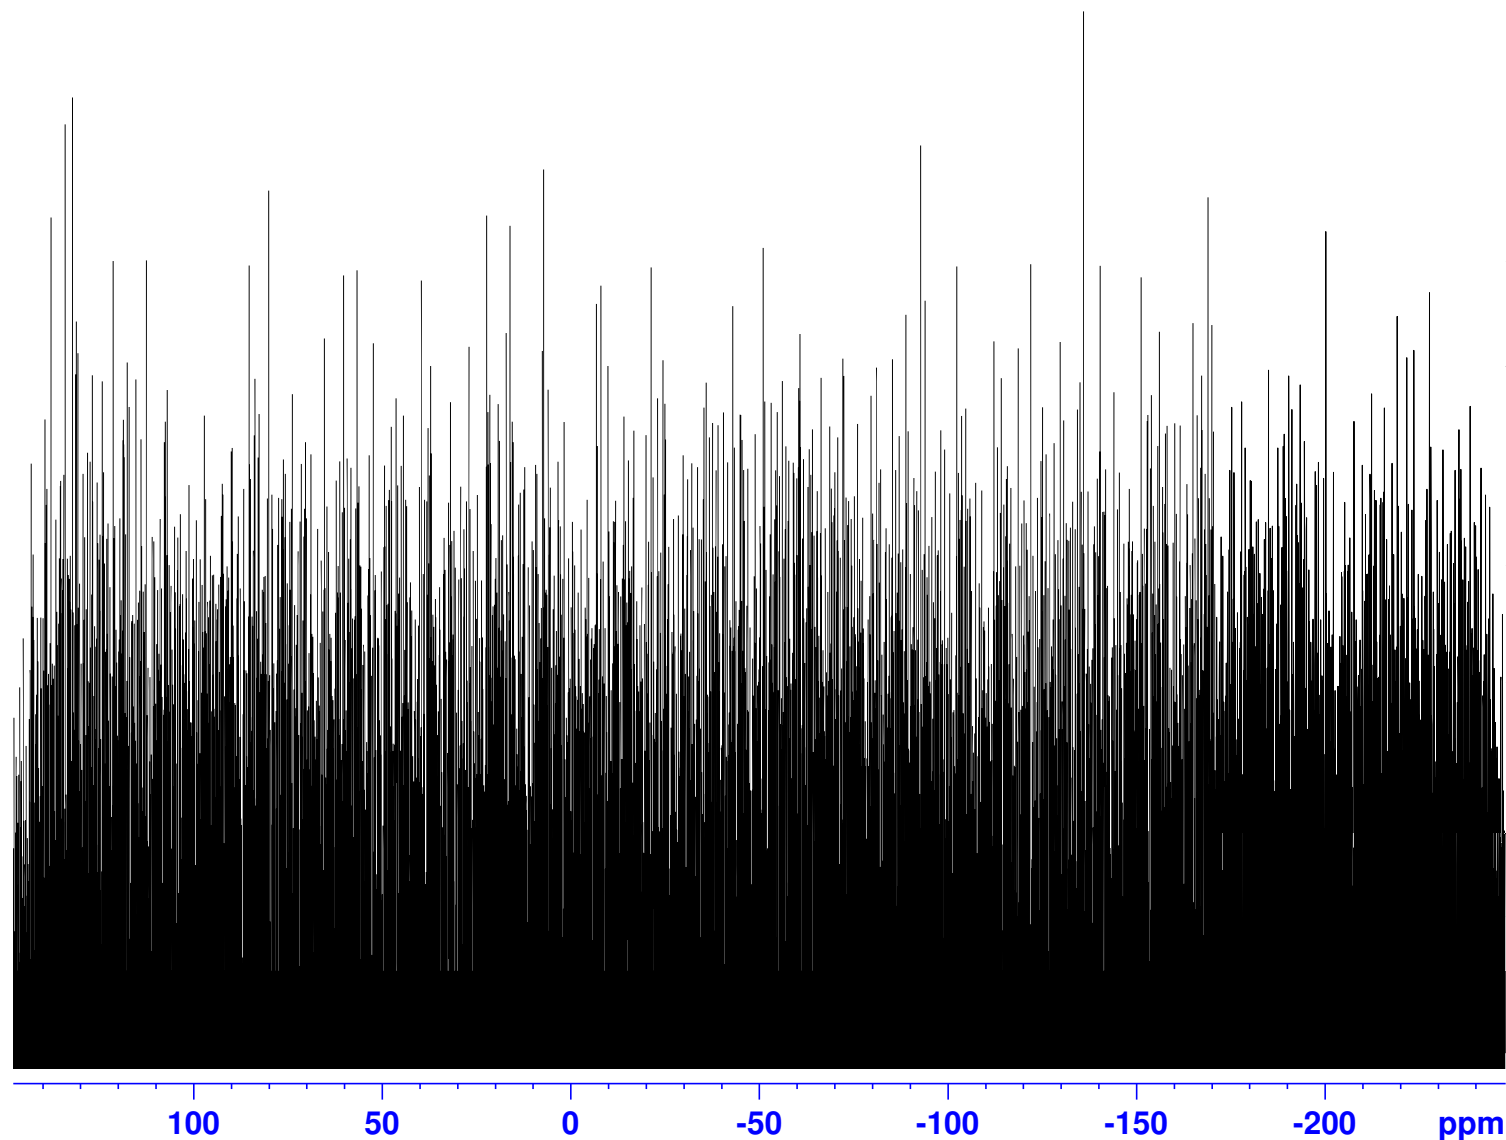

Current Data Parameters
NAME X_20180921
EXPNO 132
PROCNO 1

F2 - Acquisition Parameters
Date_ 20180921
Time 14.41 h
INSTRUM spect
PROBHD Z824801_0046 (
PULPROG zgpg30
TD 65536
SOLVENT CDC13
NS 16
DS 4
SWH 64102.562 Hz
FIDRES 1.956255 Hz
AQ 0.5111808 sec
RG 200.25
DW 7.800 usec
DE 6.50 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 162.0079729 MHz
NUC1 31P
P0 2.67 usec
P1 8.00 usec
PLW1 36.45100021 W
SFO2 400.2316009 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.23714000 W
PLW13 0.11928000 W

F2 - Processing parameters
SI 32768
SF 162.0160737 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

1.44
1.82
0.55
0.57
1.73
1.46
3.56
1.65
0.11
1.72
0.41
1.35
0.22
1.03
0.93
1.89
0.68
1.07
0.86
1.44
0.67
0.81
0.28
1.19
0.48
0.85
1.69
1.13
1.17
1.45
0.70
0.75
1.87
1.15
1.19
1.22
0.64
1.01
0.50
1.04
0.11
1.06
1.03
1.10
1.37
0.98