


aneesah akram pure analogue  
P31CPD CDC13 /opt/data Adv\_Exp 39

29.41  
27.48  
26.57  
-15.49

Current Data Parameters  
NAME X\_20180921  
EXPNO 22  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20180921  
Time 10.38 h  
INSTRUM spect  
PROBHD Z824801\_0046 (  
PULPROG zgpg30  
TD 65536  
SOLVENT CDC13  
NS 16  
DS 4  
SWH 64102.562 Hz  
FIDRES 1.956255 Hz  
AQ 0.5111808 sec  
RG 200.25  
DW 7.800 usec  
DE 6.50 usec  
TE 300.0 K  
D1 2.00000000 sec  
D11 0.03000000 sec  
TD0 1  
SFO1 162.0079729 MHz  
NUC1 31P  
P0 2.67 usec  
P1 8.00 usec  
PLW1 36.45100021 W  
SFO2 400.2316009 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 20.00000000 W  
PLW12 0.23714000 W  
PLW13 0.11928000 W

F2 - Processing parameters  
SI 32768  
SF 162.0160737 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40

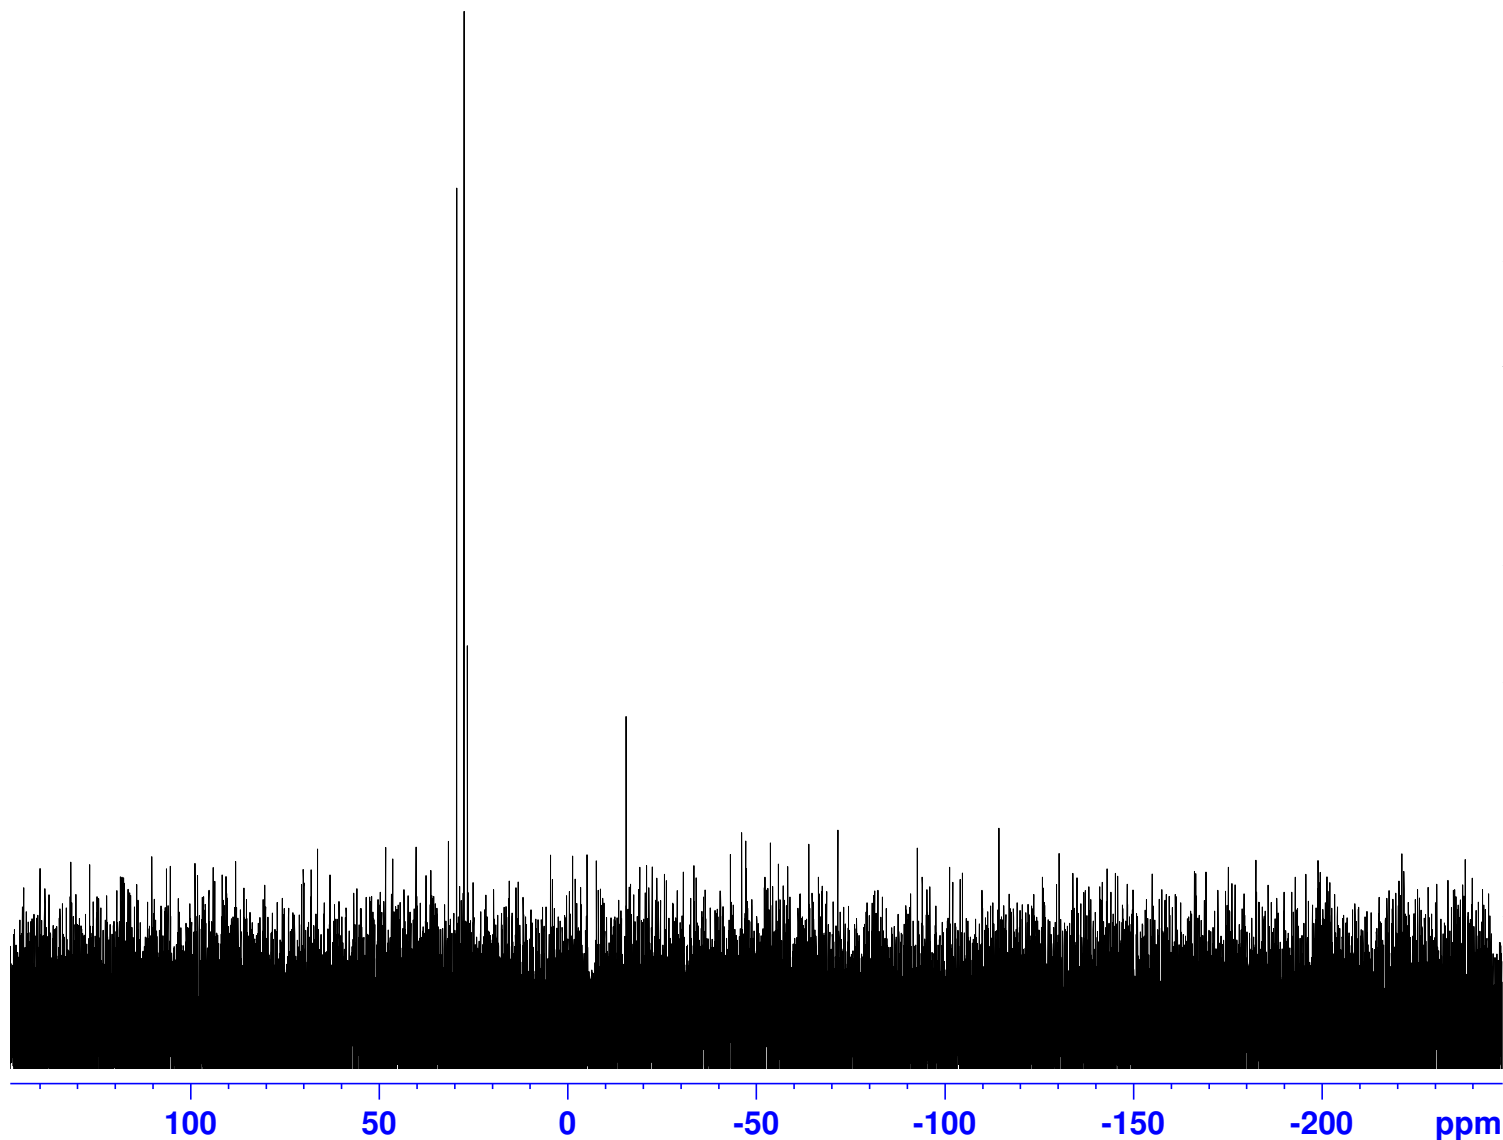

1.48  
1.70  
0.84  
0.01  
0.61  
1.52  
1.57  
0.64  
5.64  
5.92  
2.26  
1.32  
1.91  
1.80  
1.89  
0.73  
0.22  
0.86  
0.21  
0.06  
1.69  
0.79  
0.58  
1.41  
2.36  
2.74  
0.74  
0.75  
0.49  
0.62  
0.74  
0.69  
1.14  
0.95  
1.39  
0.84  
0.80  
0.60  
0.45  
0.08  
0.18  
0.08  
1.11  
0.30  
1.18