


hd02-pure comp/a
P31CPD CDC13 /opt/data Adv_Exp 3

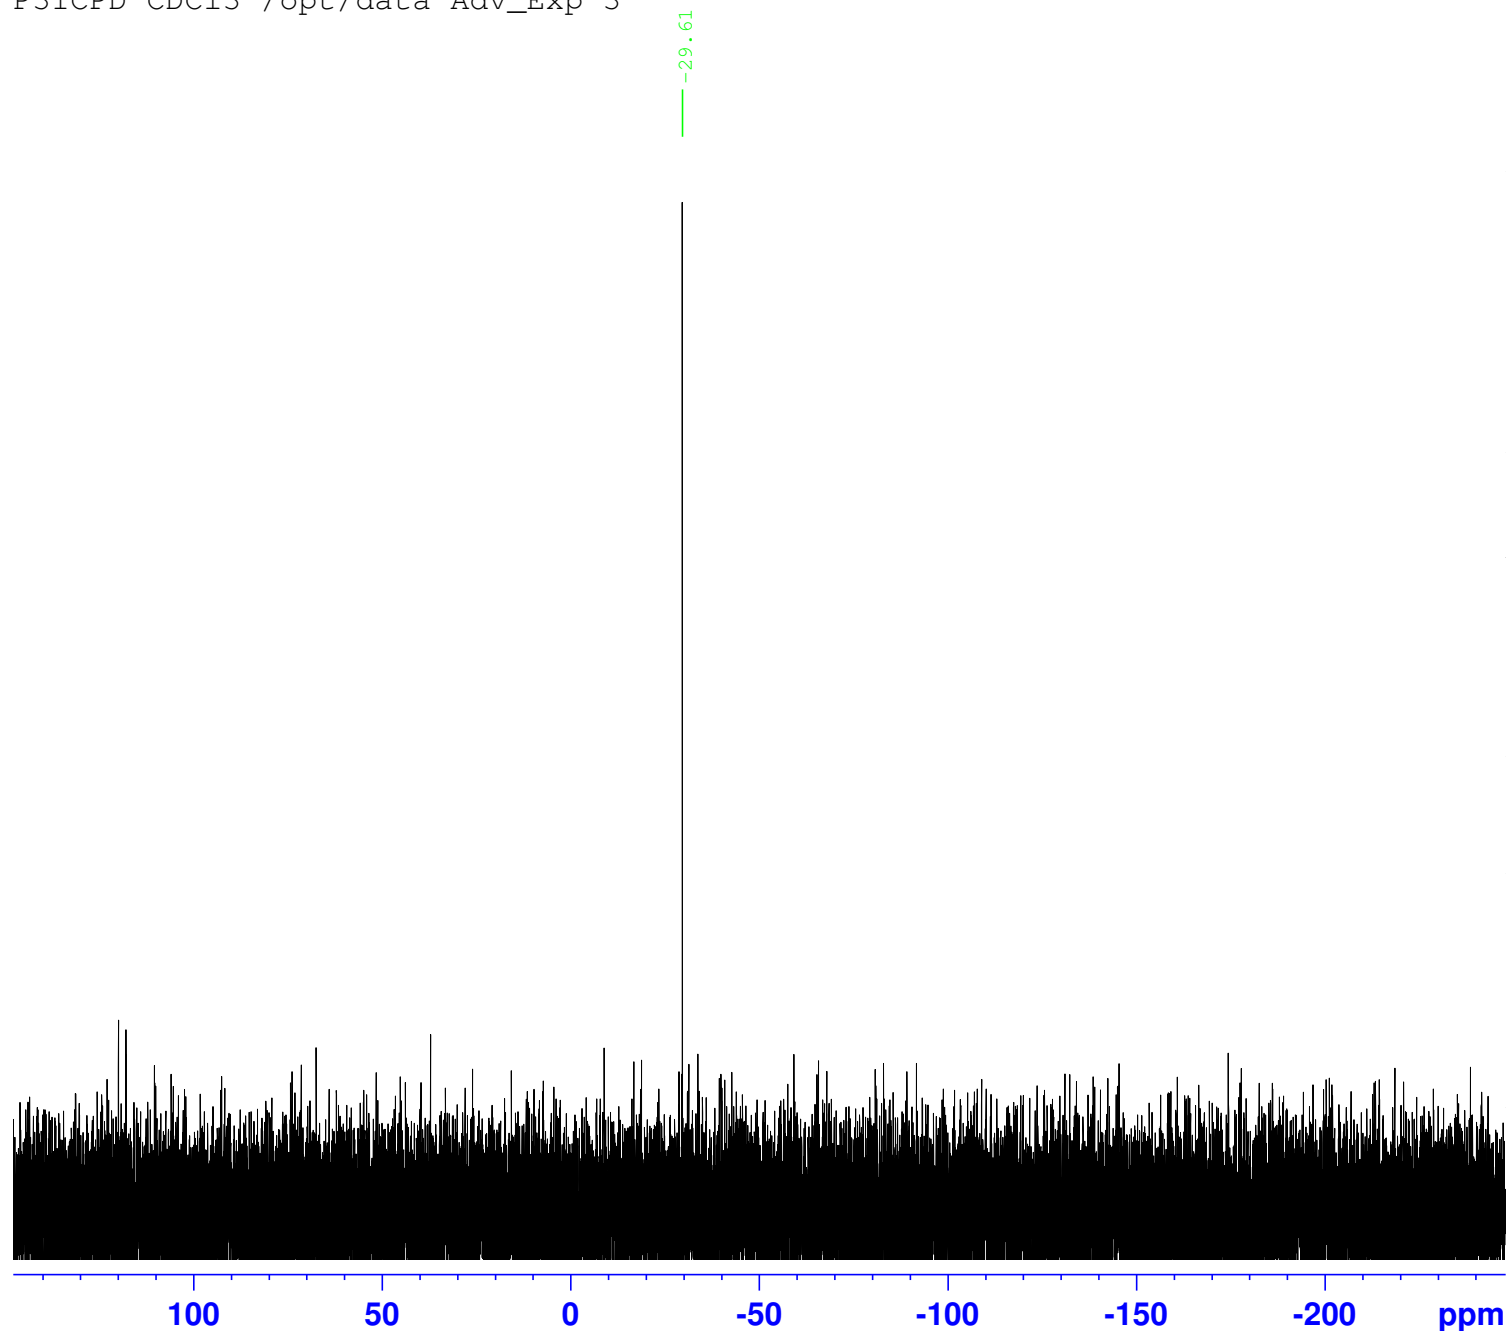

Current Data Parameters
NAME X_20181012
EXPNO 22
PROCNO 1

F2 - Acquisition Parameters
Date_ 20181012
Time 13.41 h
INSTRUM spect
PROBHD Z824801_0046 (
PULPROG zgpg30
TD 65536
SOLVENT CDC13
NS 16
DS 4
SWH 64102.562 Hz
FIDRES 1.956255 Hz
AQ 0.5111808 sec
RG 200.25
DW 7.800 usec
DE 6.50 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 162.0079729 MHz
NUC1 31P
P0 2.67 usec
P1 8.00 usec
PLW1 36.45100021 W
SFO2 400.2316009 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.23714000 W
PLW13 0.11928000 W

F2 - Processing parameters
SI 32768
SF 162.0160737 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

1.43
1.36
1.32
0.64
1.33
1.59
0.68
0.29
1.08
1.66
0.44
0.15
0.62
0.95
0.92
2.06
6.18
2.54
0.53
2.10
1.16
1.22
1.36
1.71
1.08
0.24
3.28
2.60
0.66
1.67
0.95
0.65
0.83
1.22
1.00
0.06
0.73
1.09
0.08
0.98
1.01
0.72
1.39
0.94
1.35
1.99
1.36