


BB08 - Compound 3  
P31CPD CDCl3 /opt/data Adv\_Exp 17

33.14  
23.97

Current Data Parameters  
NAME X\_20181106  
EXPNO 281  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20181107  
Time 8.29 h  
INSTRUM spect  
PROBHD Z824801\_0046 (  
PULPROG zgpg30  
TD 65536  
SOLVENT CDCl3  
NS 16  
DS 4  
SWH 64102.562 Hz  
FIDRES 1.956255 Hz  
AQ 0.5111808 sec  
RG 200.25  
DW 7.800 usec  
DE 6.50 usec  
TE 300.0 K  
D1 2.00000000 sec  
D11 0.03000000 sec  
TD0 1  
SFO1 162.0079729 MHz  
NUC1 31P  
P0 2.67 usec  
P1 8.00 usec  
PLW1 36.45100021 W  
SFO2 400.2316009 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 20.00000000 W  
PLW12 0.23714000 W  
PLW13 0.11928000 W

F2 - Processing parameters  
SI 32768  
SF 162.0160737 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40

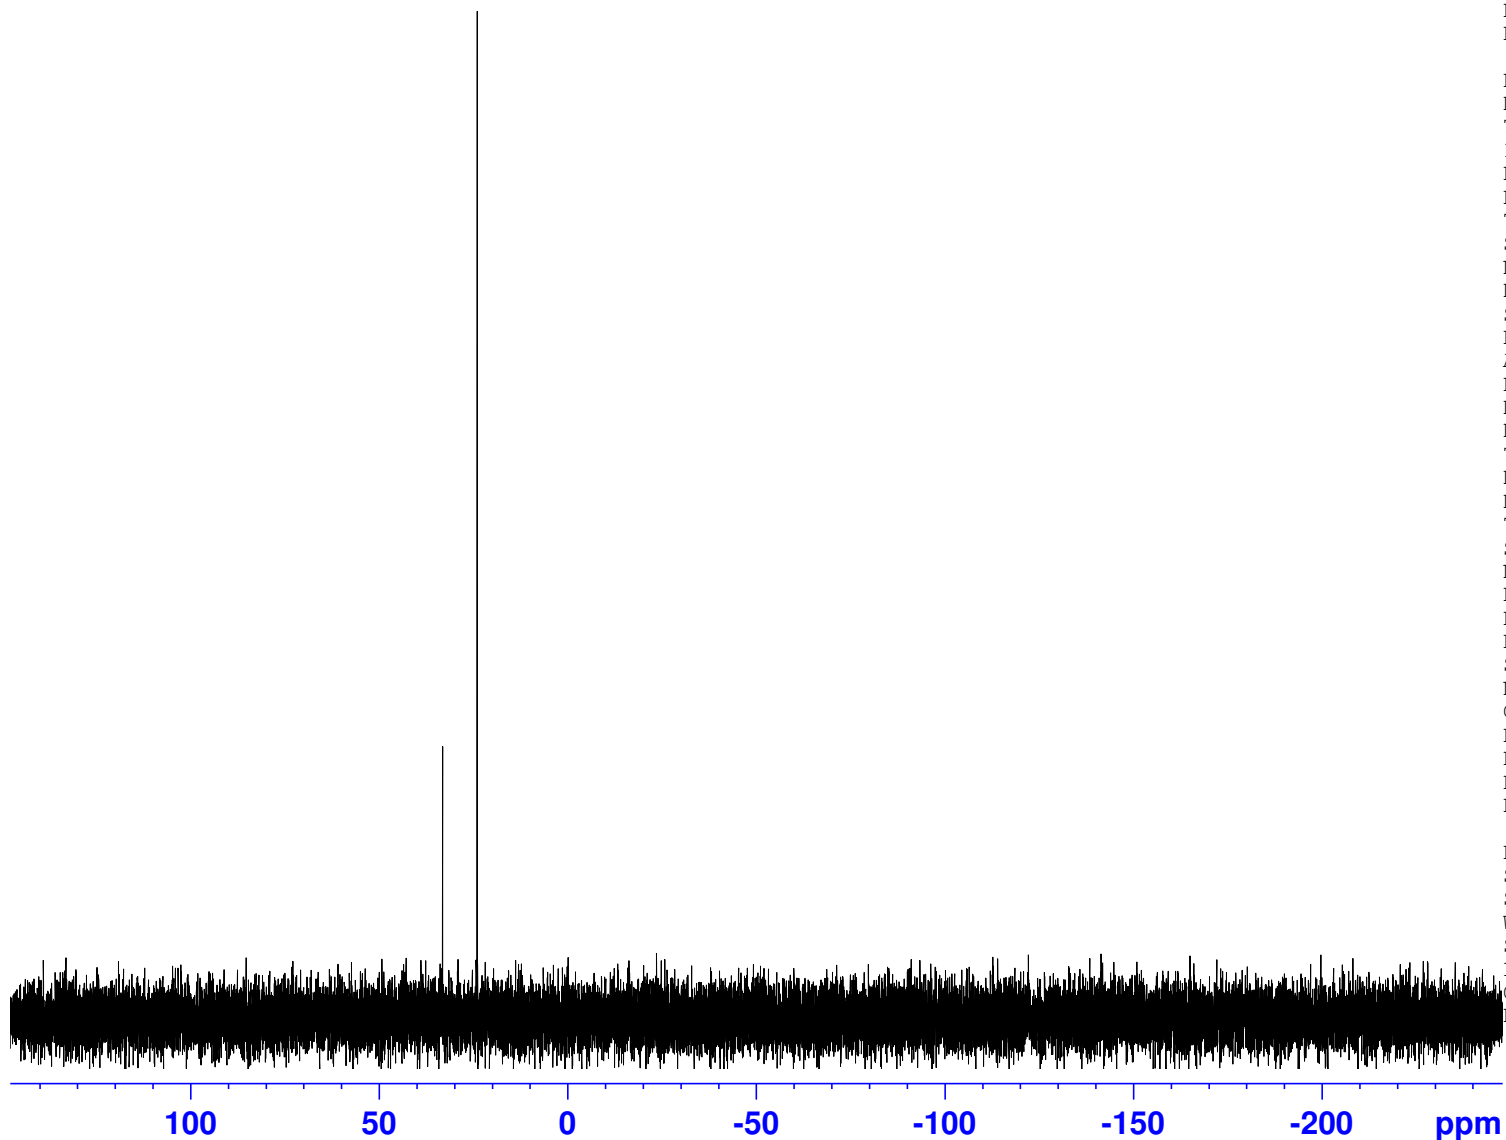

2.30 1.07 3.93 2.14 2.21 2.81 7.79 1.05 0.65 0.84 1.25 0.52 1.15 0.71 0.69 1.01 1.49 1.53 0.99 0.13 0.28 0.97 0.50 0.09 0.84 1.41 0.75 0.05 0.80 1.35 0.37 1.72 0.34 0.68 2.30 0.92 0.57 0.78 0.28 1.44 0.21 2.32 1.93 0.99 2.43 0.50