


CHE311 AP1H  
P31CPD CDCl3 /opt/data Adv\_Exp 27

23.23

Current Data Parameters  
NAME X\_20181106  
EXPNO 301  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20181107  
Time 9.03 h  
INSTRUM spect  
PROBHD Z824801\_0046 (  
PULPROG zgpg30  
TD 65536  
SOLVENT CDCl3  
NS 16  
DS 4  
SWH 64102.562 Hz  
FIDRES 1.956255 Hz  
AQ 0.5111808 sec  
RG 200.25  
DW 7.800 usec  
DE 6.50 usec  
TE 300.0 K  
D1 2.00000000 sec  
D11 0.03000000 sec  
TD0 1  
SFO1 162.0079729 MHz  
NUC1 31P  
P0 2.67 usec  
P1 8.00 usec  
PLW1 36.45100021 W  
SFO2 400.2316009 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 20.00000000 W  
PLW12 0.23714000 W  
PLW13 0.11928000 W

F2 - Processing parameters  
SI 32768  
SF 162.0160737 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40

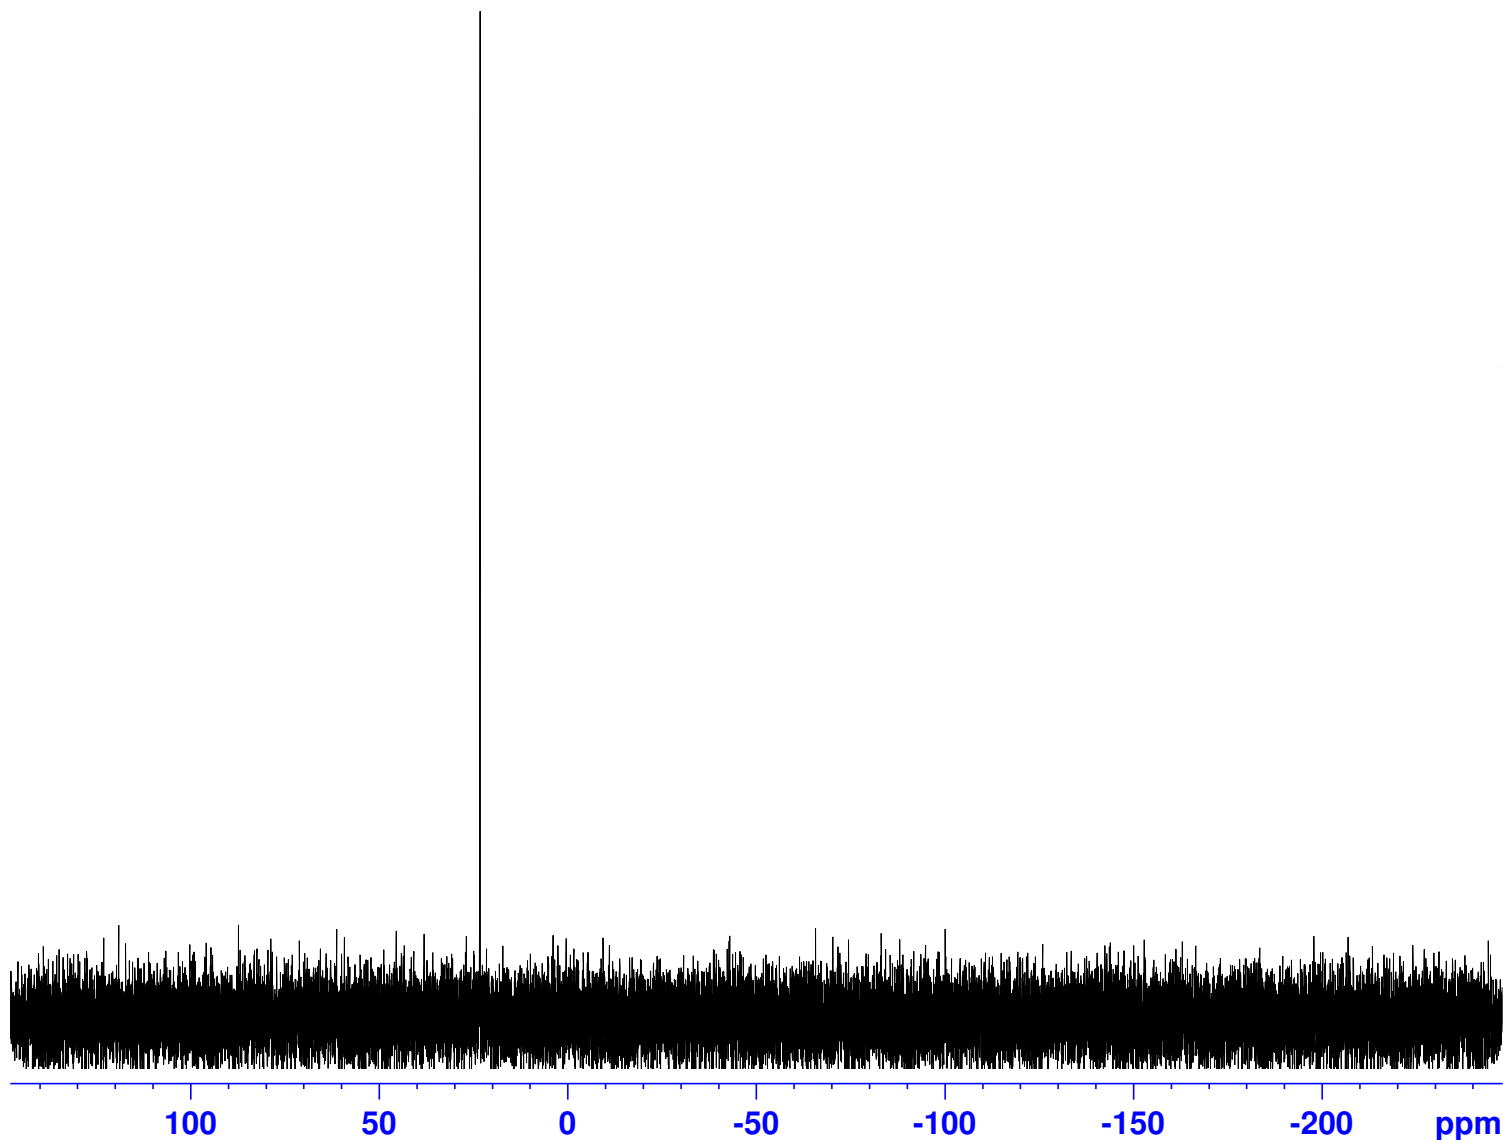

1.02 1.02 1.42 1.09 0.99 1.32 1.48 0.09 6.15 0.70 1.57 1.21 0.77 1.29 1.07 0.49 0.09 0.68 0.08 0.38 0.90 0.29 1.04 0.70 0.64 0.91 0.90 0.12 1.02 0.41 1.20 0.47 1.87 0.11 0.10 0.80 1.82 0.18 1.32 0.10 0.67 0.84 0.85 1.48 1.27 1.86