


CHE311 AP4H
P31CPD CDC13 /opt/data Adv_Exp 28

Current Data Parameters
NAME X_20181106
EXPNO 311
PROCNO 1

F2 - Acquisition Parameters
Date_ 20181107
Time 9.09 h
INSTRUM spect
PROBHD Z824801_0046 (
PULPROG zgpg30
TD 65536
SOLVENT CDC13
NS 16
DS 4
SWH 64102.562 Hz
FIDRES 1.956255 Hz
AQ 0.5111808 sec
RG 200.25
DW 7.800 usec
DE 6.50 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 162.0079729 MHz
NUC1 31P
P0 2.67 usec
P1 8.00 usec
PLW1 36.45100021 W
SFO2 400.2316009 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.23714000 W
PLW13 0.11928000 W

F2 - Processing parameters
SI 32768
SF 162.0160737 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

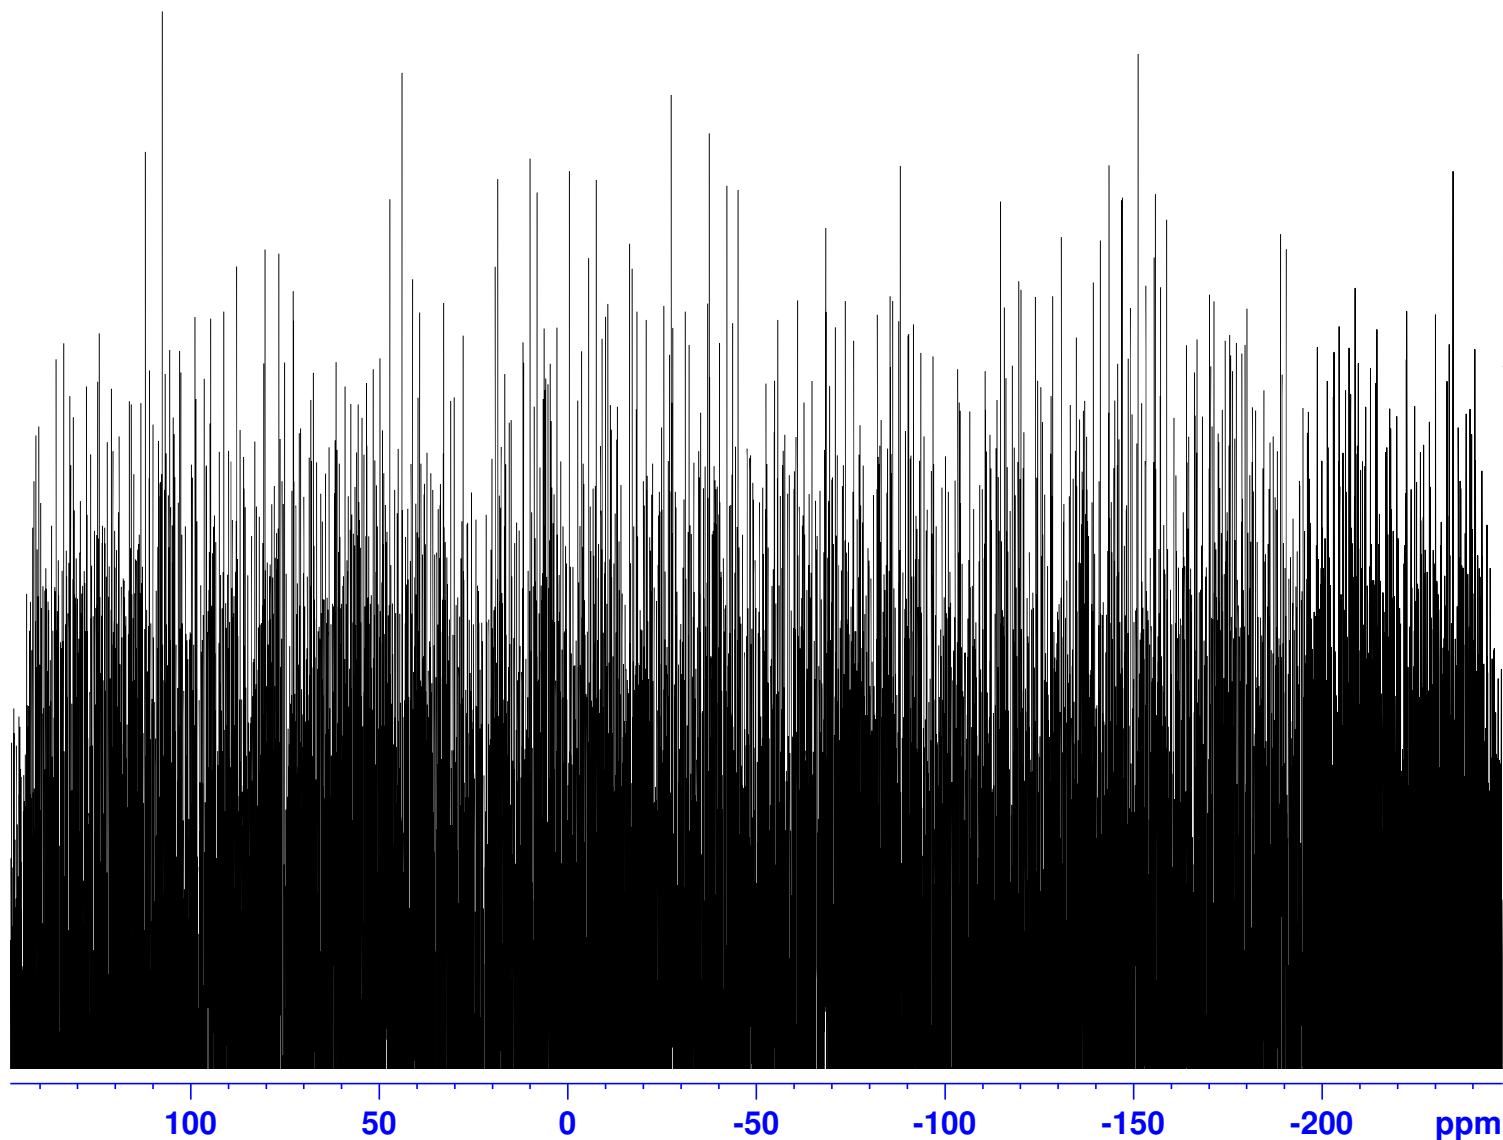

0.77
0.85
1.48
0.18
1.71
0.82
0.08
1.29
0.90
1.37
1.52
0.70
2.15
1.26
0.61
0.43
1.87
1.73
1.37
1.48
1.33
0.90
1.16
1.78
1.77
0.37
1.79
0.79
0.29
0.96
0.15
1.32
0.51
0.67
1.96
1.18
0.90
0.61
1.45
1.57
1.81
1.78
0.94
0.67
1.93
2.04
1.16