


PRK 1H compound 4
P31CPD CDCl3 /opt/data Adv_Exp 48

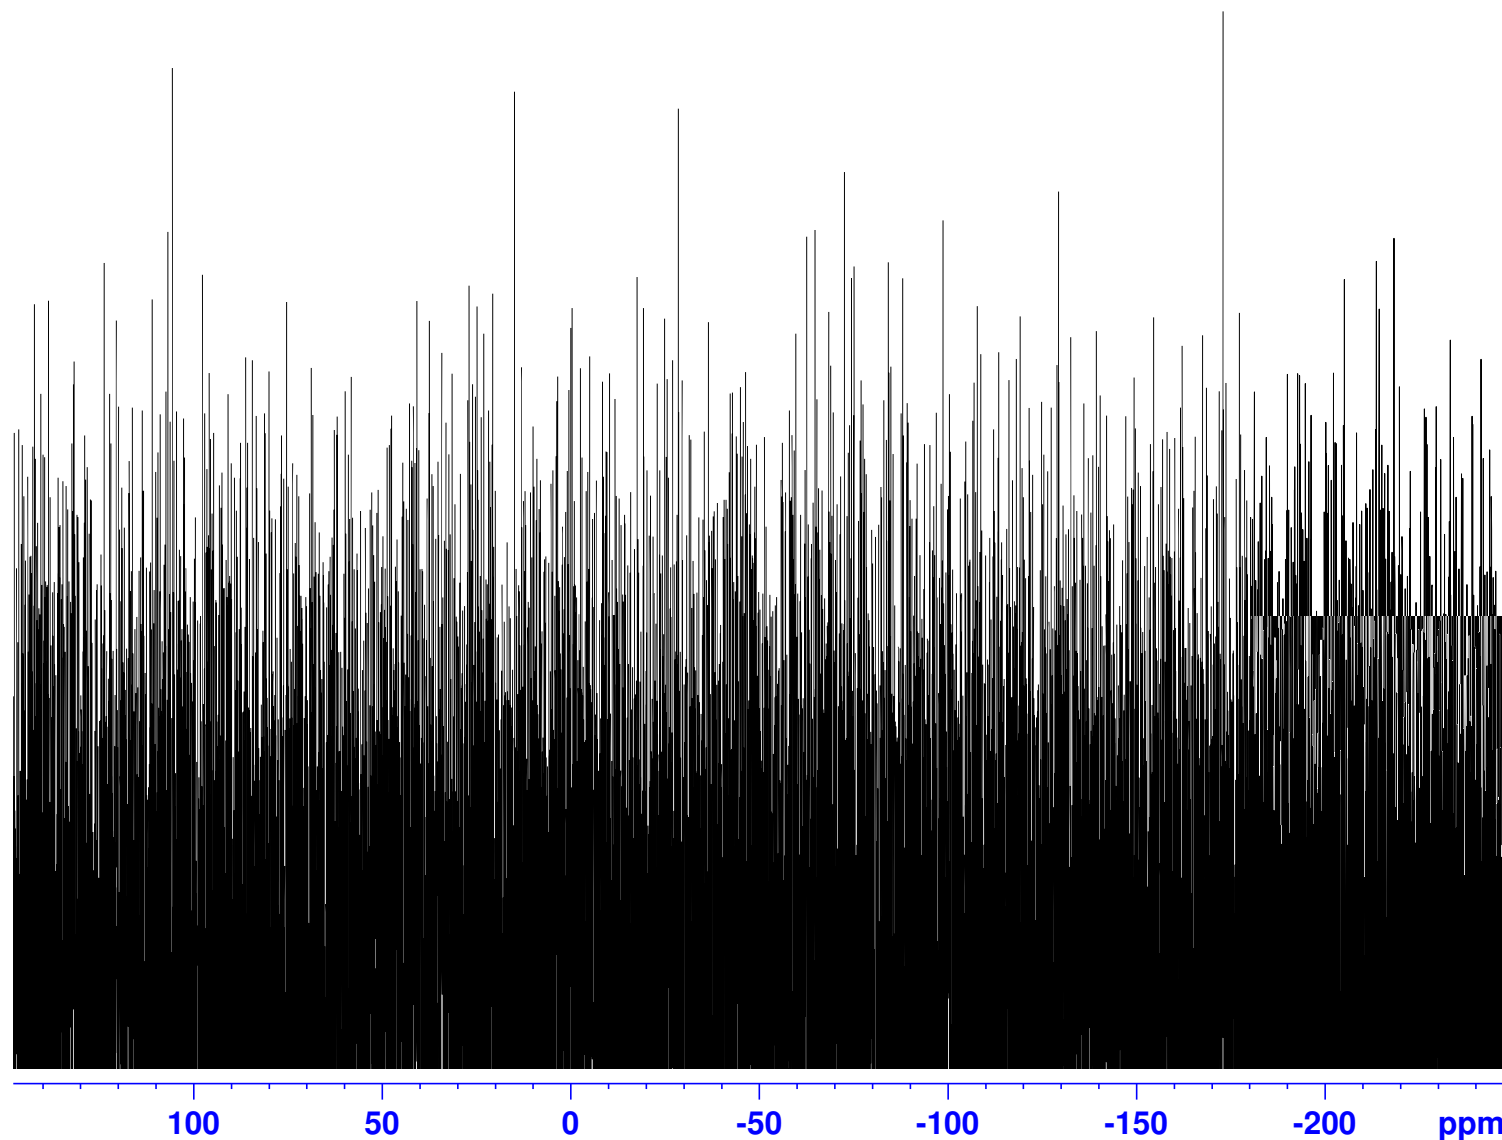

Current Data Parameters
NAME X_20181106
EXPNO 351
PROCNO 1

F2 - Acquisition Parameters
Date_ 20181106
Time 17.39 h
INSTRUM spect
PROBHD Z824801_0046 (
PULPROG zgpg30
TD 65536
SOLVENT CDCl3
NS 16
DS 4
SWH 64102.562 Hz
FIDRES 1.956255 Hz
AQ 0.5111808 sec
RG 200.25
DW 7.800 usec
DE 6.50 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 162.0079729 MHz
NUC1 31P
P0 2.67 usec
P1 8.00 usec
PLW1 36.45100021 W
SFO2 400.2316009 MHz
NUC2 1H
CPDPRG2 waltz16
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.23714000 W
PLW13 0.11928000 W

F2 - Processing parameters
SI 32768
SF 162.0160737 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

1.65
0.31
1.29
1.01
1.82
0.84
1.02
1.96
1.67
0.06
0.00
0.31
1.25
1.65
1.16
0.33
0.59
1.55
2.07
1.38
0.77
1.02
0.85
0.73
3.06
1.30
1.45
1.39
1.68
0.54
1.21
1.21
0.91
0.10
1.09
1.62
2.21
0.12
1.72
1.28
0.15
1.22
0.28
1.10
1.04
1.52