


che311 AP 1st product  
P31CPD CDCl3 /opt/data Adv\_Exp 41

29.09  
-5.33

Current Data Parameters  
NAME X\_20181107  
EXPNO 212  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20181108  
Time 6.04 h  
INSTRUM spect  
PROBHD Z824801\_0046 (  
PULPROG zgpg30  
TD 65536  
SOLVENT CDCl3  
NS 16  
DS 4  
SWH 64102.562 Hz  
FIDRES 1.956255 Hz  
AQ 0.5111808 sec  
RG 200.25  
DW 7.800 usec  
DE 6.50 usec  
TE 300.0 K  
D1 2.00000000 sec  
D11 0.03000000 sec  
TD0 1  
SFO1 162.0079729 MHz  
NUC1 31P  
P0 2.67 usec  
P1 8.00 usec  
PLW1 36.45100021 W  
SFO2 400.2316009 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 20.00000000 W  
PLW12 0.23714000 W  
PLW13 0.11928000 W

F2 - Processing parameters  
SI 32768  
SF 162.0160737 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40

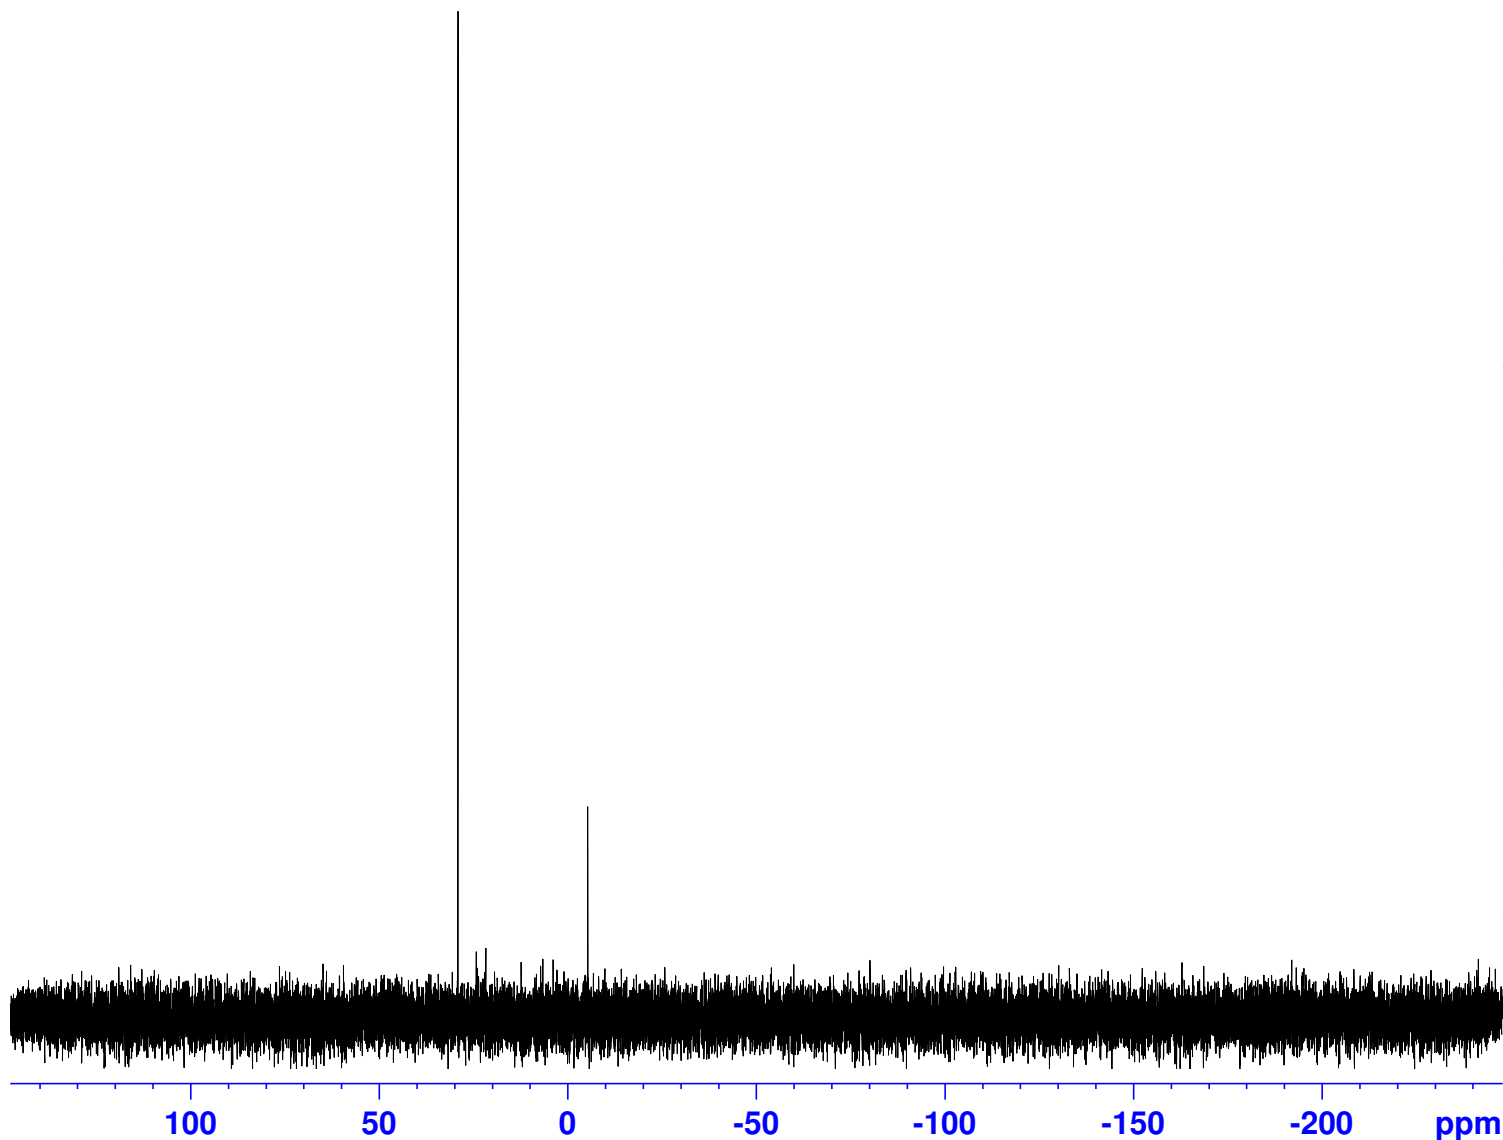

1.17  
1.45  
1.23  
0.72  
1.36  
3.90  
0.67  
3.14  
2.01  
3.54  
1.09  
0.23  
0.50  
0.50  
0.01  
4.42  
0.43  
1.12  
0.73  
0.17  
0.80  
0.60  
1.47  
1.10  
1.58  
1.28  
1.02  
1.23  
0.46  
0.68  
1.01  
0.62  
1.01  
2.95  
0.59  
1.28  
0.43  
1.54  
3.17  
1.26  
0.70  
1.49  
0.58  
1.08  
1.57  
0.79