


ws13  
P31CPD CDC13 /opt/data SAWS 5

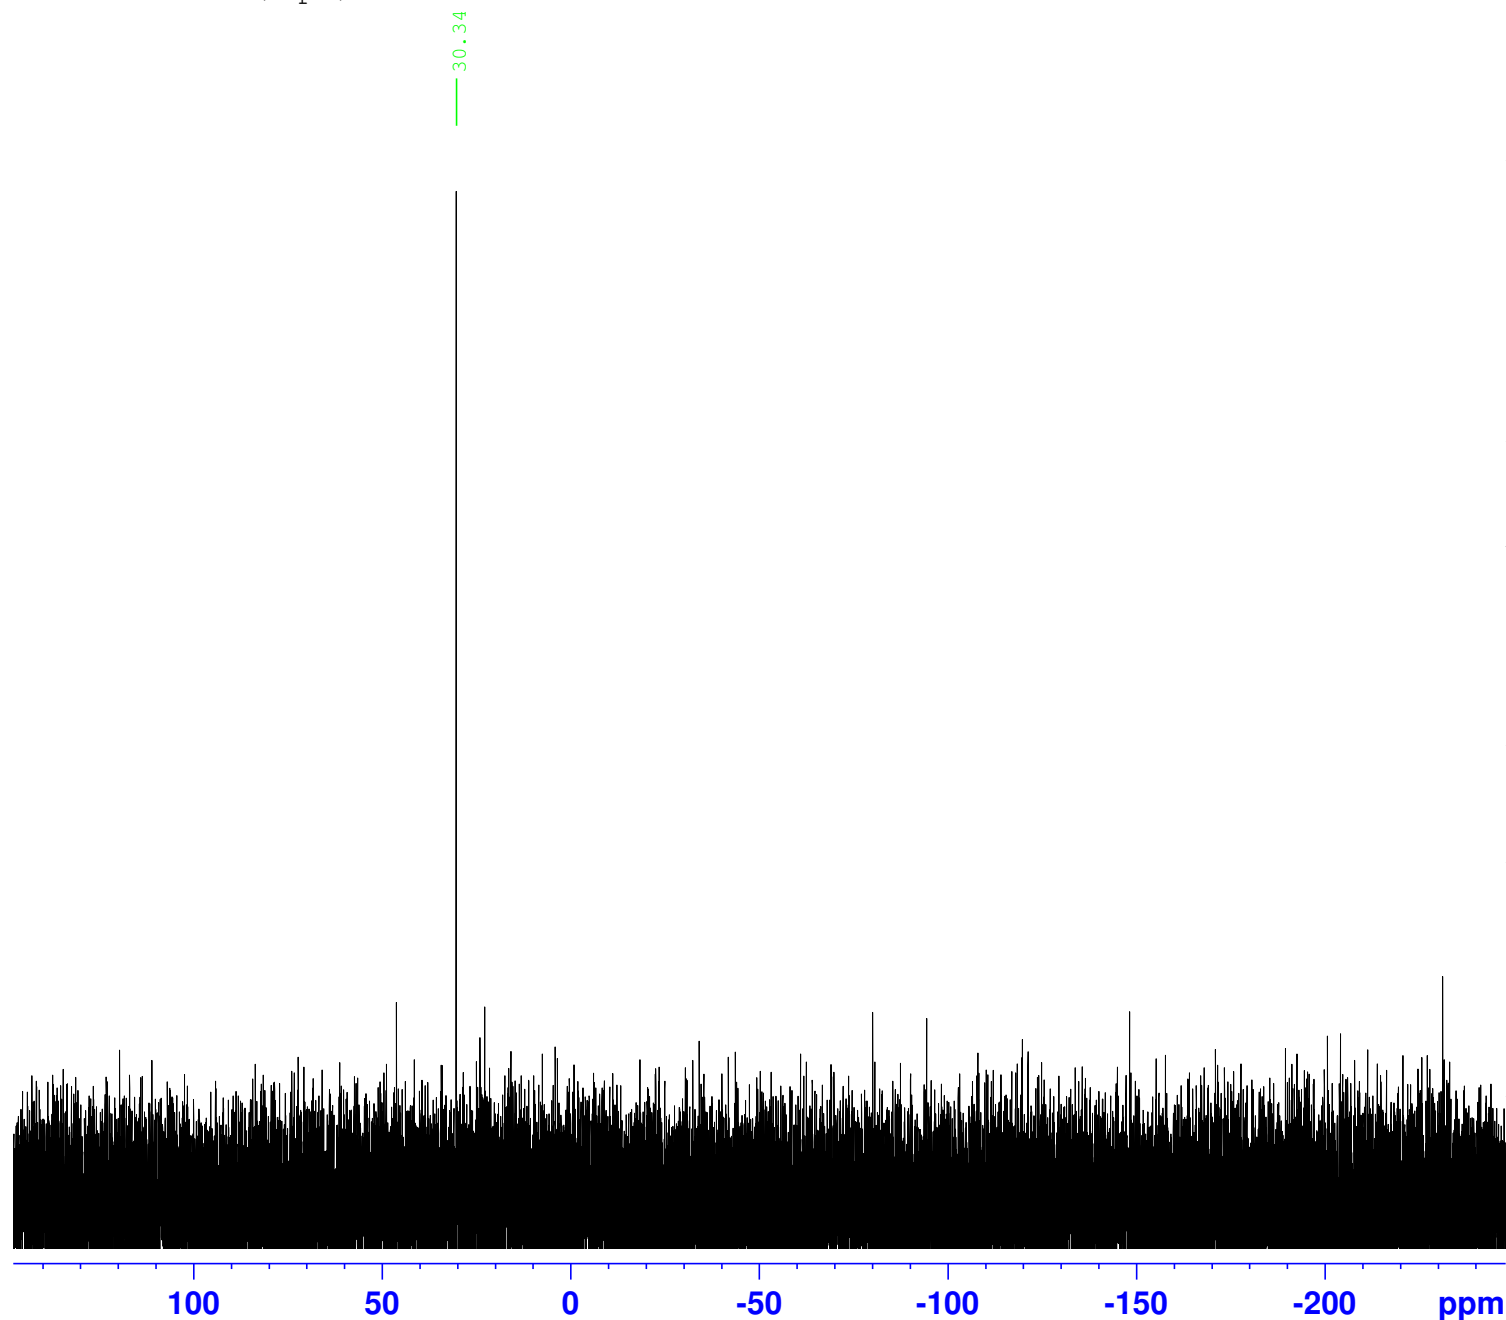

Current Data Parameters  
NAME X\_20181107  
EXPNO 251  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20181107  
Time 14.08 h  
INSTRUM spect  
PROBHD Z824801\_0046 (  
PULPROG zgpg30  
TD 65536  
SOLVENT CDCl3  
NS 16  
DS 4  
SWH 64102.562 Hz  
FIDRES 1.956255 Hz  
AQ 0.5111808 sec  
RG 200.25  
DW 7.800 usec  
DE 6.50 usec  
TE 300.0 K  
D1 2.00000000 sec  
D11 0.03000000 sec  
TD0 1  
SFO1 162.0079729 MHz  
NUC1 31P  
P0 2.67 usec  
P1 8.00 usec  
PLW1 36.45100021 W  
SFO2 400.2316009 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 20.00000000 W  
PLW12 0.23714000 W  
PLW13 0.11928000 W

F2 - Processing parameters  
SI 32768  
SF 162.0160737 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40

1.03 1.28 0.56 0.62 0.88 1.80 1.95 1.30 3.10 0.63 1.23 0.92 0.74 1.91 2.53 1.75 0.10 0.94 1.31 0.77 1.80 1.14 0.40 1.74 0.91 1.39 0.65 1.32 1.19 1.68 0.32 1.46 2.11 1.26 0.20 1.16 0.84 0.52 1.97 1.34 1.78 0.73 1.45 1.77 0.64 1.57