


PT3  
P31CPD CDC13 /opt/data Adv\_Exp 17

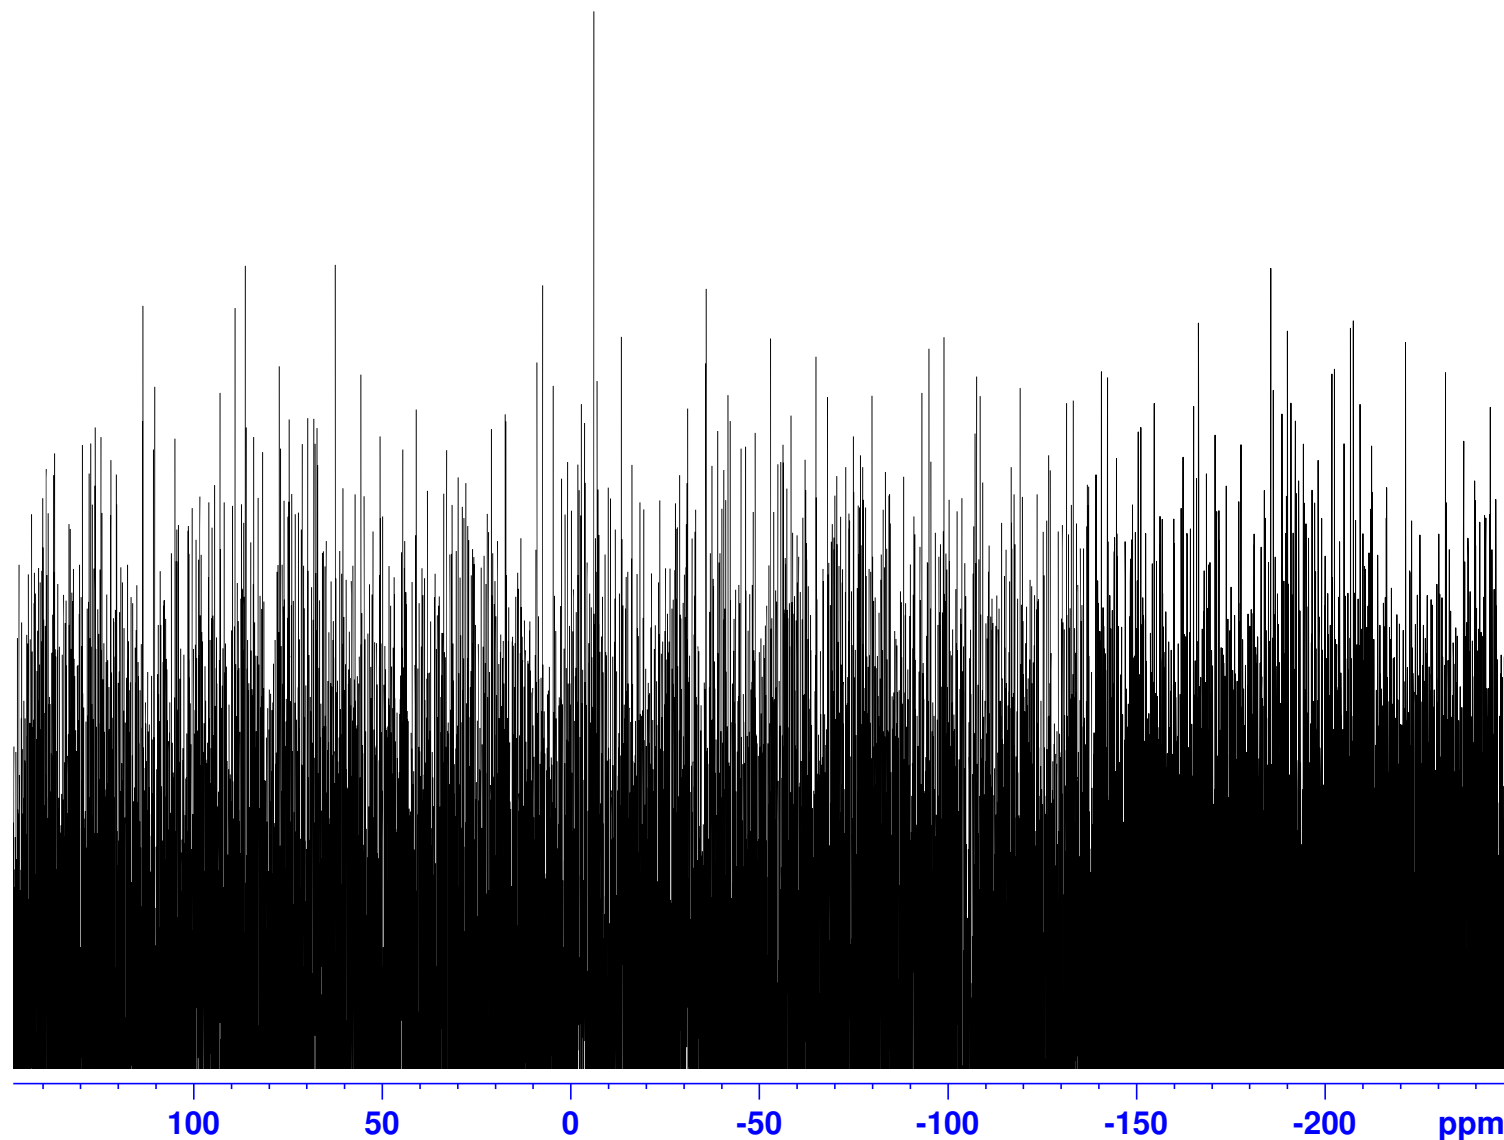

Current Data Parameters  
NAME X\_20181107  
EXPNO 442  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20181108  
Time 18.19 h  
INSTRUM spect  
PROBHD Z824801\_0046 (  
PULPROG zgpg30  
TD 65536  
SOLVENT CDC13  
NS 16  
DS 4  
SWH 64102.562 Hz  
FIDRES 1.956255 Hz  
AQ 0.5111808 sec  
RG 200.25  
DW 7.800 usec  
DE 6.50 usec  
TE 300.0 K  
D1 2.00000000 sec  
D11 0.03000000 sec  
TD0 1  
SFO1 162.0079729 MHz  
NUC1 31P  
P0 2.67 usec  
P1 8.00 usec  
PLW1 36.45100021 W  
SFO2 400.2316009 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 20.00000000 W  
PLW12 0.23714000 W  
PLW13 0.11928000 W

F2 - Processing parameters  
SI 32768  
SF 162.0160737 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40

1.93 1.42 0.08 0.24 1.55 1.66 0.15 1.29 1.01 0.94 2.42 1.54 0.35 1.13 1.25 1.88 2.99 0.35 0.78 1.19 0.30 2.68 1.32 1.88 1.94 1.12 1.36 0.57 1.26 4.45 0.36 2.31 1.43 1.10 1.29 1.17 0.37 1.96 0.80 0.05 1.37 1.15 0.70 1.50 2.66