


PT4  
P31CPD CDC13 /opt/data Adv\_Exp 18

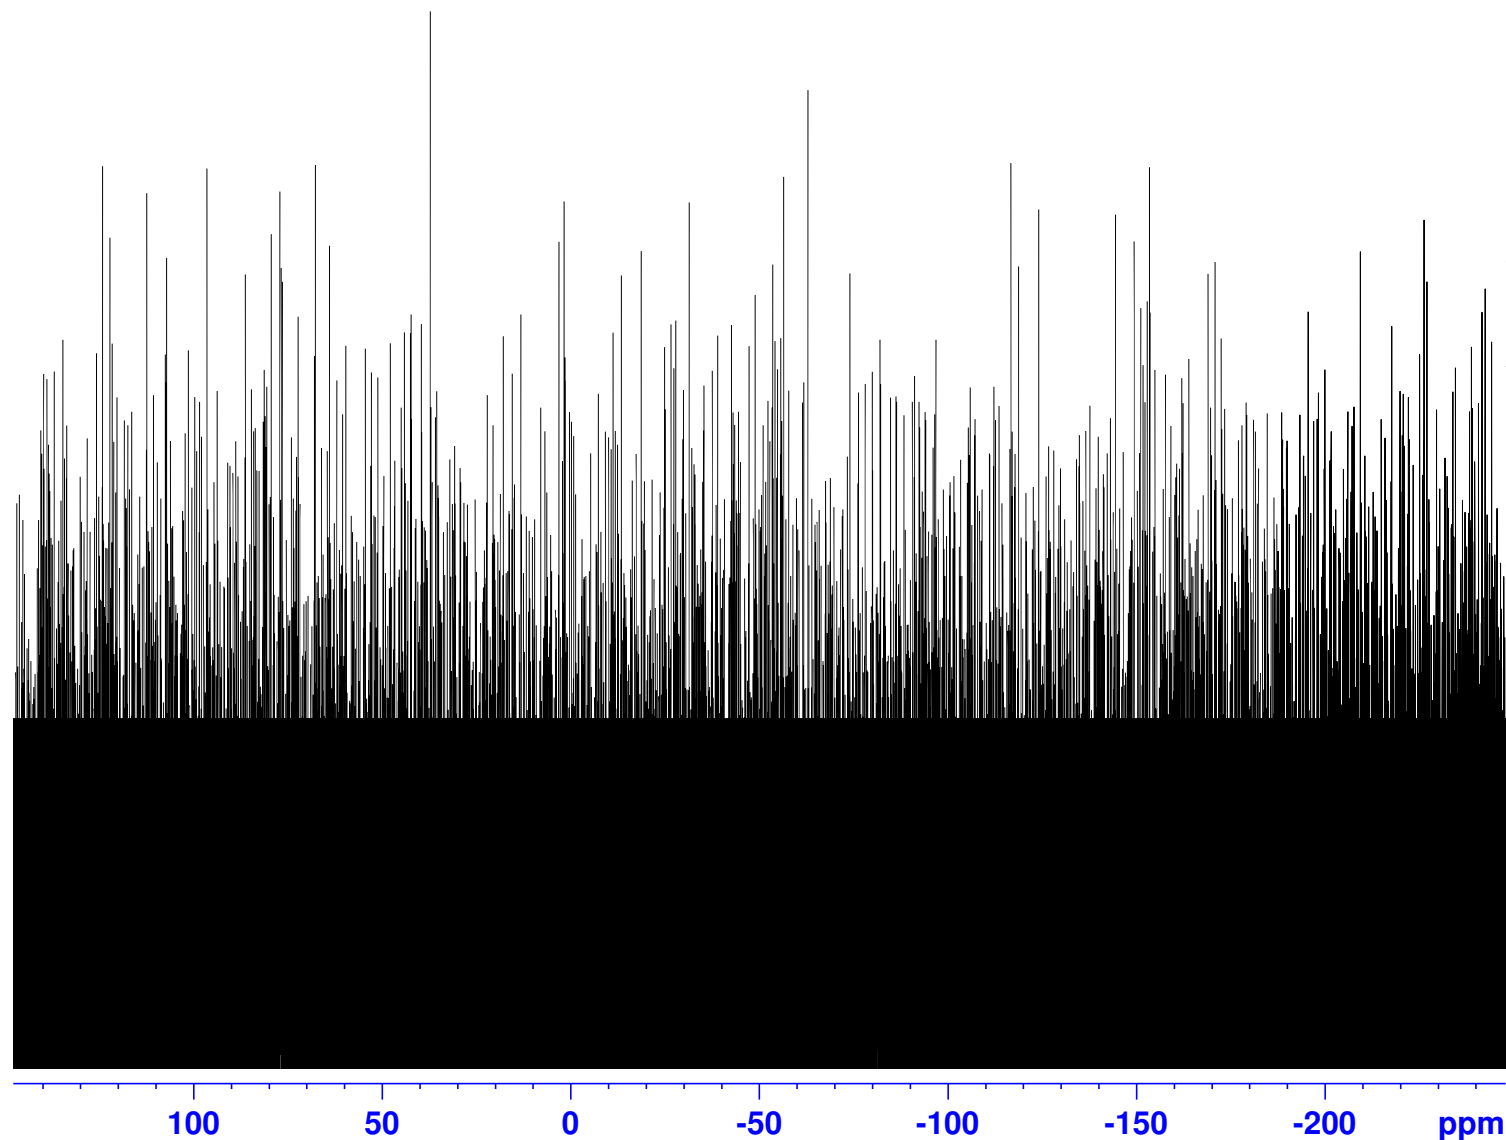

Current Data Parameters  
NAME X\_20181107  
EXPNO 452  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20181108  
Time 18.44 h  
INSTRUM spect  
PROBHD Z824801\_0046 (  
PULPROG zgpg30  
TD 65536  
SOLVENT CDC13  
NS 16  
DS 4  
SWH 64102.562 Hz  
FIDRES 1.956255 Hz  
AQ 0.5111808 sec  
RG 200.25  
DW 7.800 usec  
DE 6.50 usec  
TE 300.0 K  
D1 2.00000000 sec  
D11 0.03000000 sec  
TD0 1  
SFO1 162.0079729 MHz  
NUC1 31P  
P0 2.67 usec  
P1 8.00 usec  
PLW1 36.45100021 W  
SFO2 400.2316009 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 20.00000000 W  
PLW12 0.23714000 W  
PLW13 0.11928000 W

F2 - Processing parameters  
SI 32768  
SF 162.0160737 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40

1.11 2.25 2.82 0.66 0.59 1.87 1.72 0.36 2.41 2.16 0.04 1.30 0.82 1.43 1.14 0.30 0.38 0.46 1.61 1.30 0.80 1.38 2.11 0.03 0.63 0.76 2.38 0.47 1.95 1.52 0.38 0.14 2.47 0.54 0.95 0.65 1.27 1.12 0.36 0.58 1.21 1.52 0.44 0.65 1.76 1.96