


PRK 1P CRUDE COMPOUND 1
P31CPD CDC13 /opt/data Adv_Exp 41

29.07
21.98

Current Data Parameters
NAME X_20181108
EXPNO 102
PROCNO 1

F2 - Acquisition Parameters
Date_ 20181109
Time 10.56 h
INSTRUM spect
PROBHD Z824801_0046 (
PULPROG zgpg30
TD 65536
SOLVENT CDC13
NS 16
DS 4
SWH 64102.562 Hz
FIDRES 1.956255 Hz
AQ 0.5111808 sec
RG 200.25
DW 7.800 usec
DE 6.50 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 162.0079729 MHz
NUC1 31P
P0 2.67 usec
P1 8.00 usec
PLW1 36.45100021 W
SFO2 400.2316009 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.23714000 W
PLW13 0.11928000 W

F2 - Processing parameters
SI 32768
SF 162.0160737 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

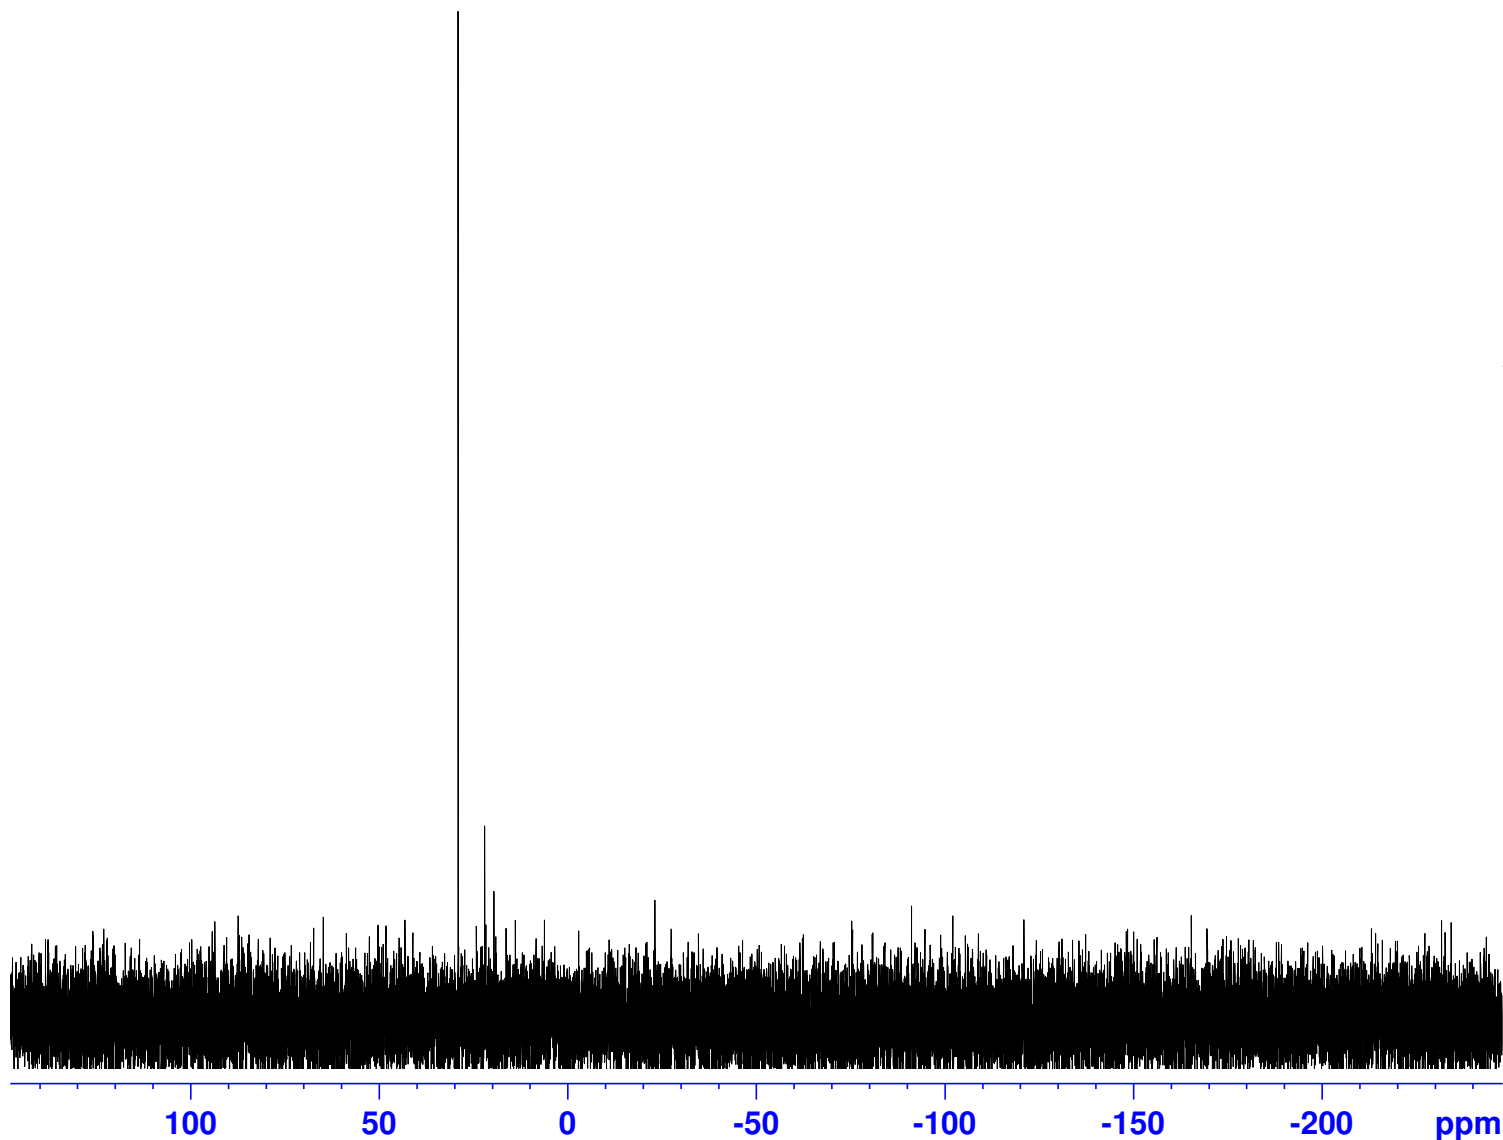

1.26
1.69
0.84
0.83
1.83
1.54
1.49
6.09
2.35
0.52
0.89
0.85
0.64
1.13
1.46
1.60
0.73
1.37
1.39
0.22
1.41
1.25
0.69
0.21
0.76
0.60
0.52
0.87
1.43
0.60
1.06
0.84
0.83
0.63
0.56
1.91
1.11
1.59
0.16
0.35
1.09
1.63
0.11
2.24
2.72
1.11