


PRK 1P COMPOUND 4
P31CPD CDC13 /opt/data Adv_Exp 1

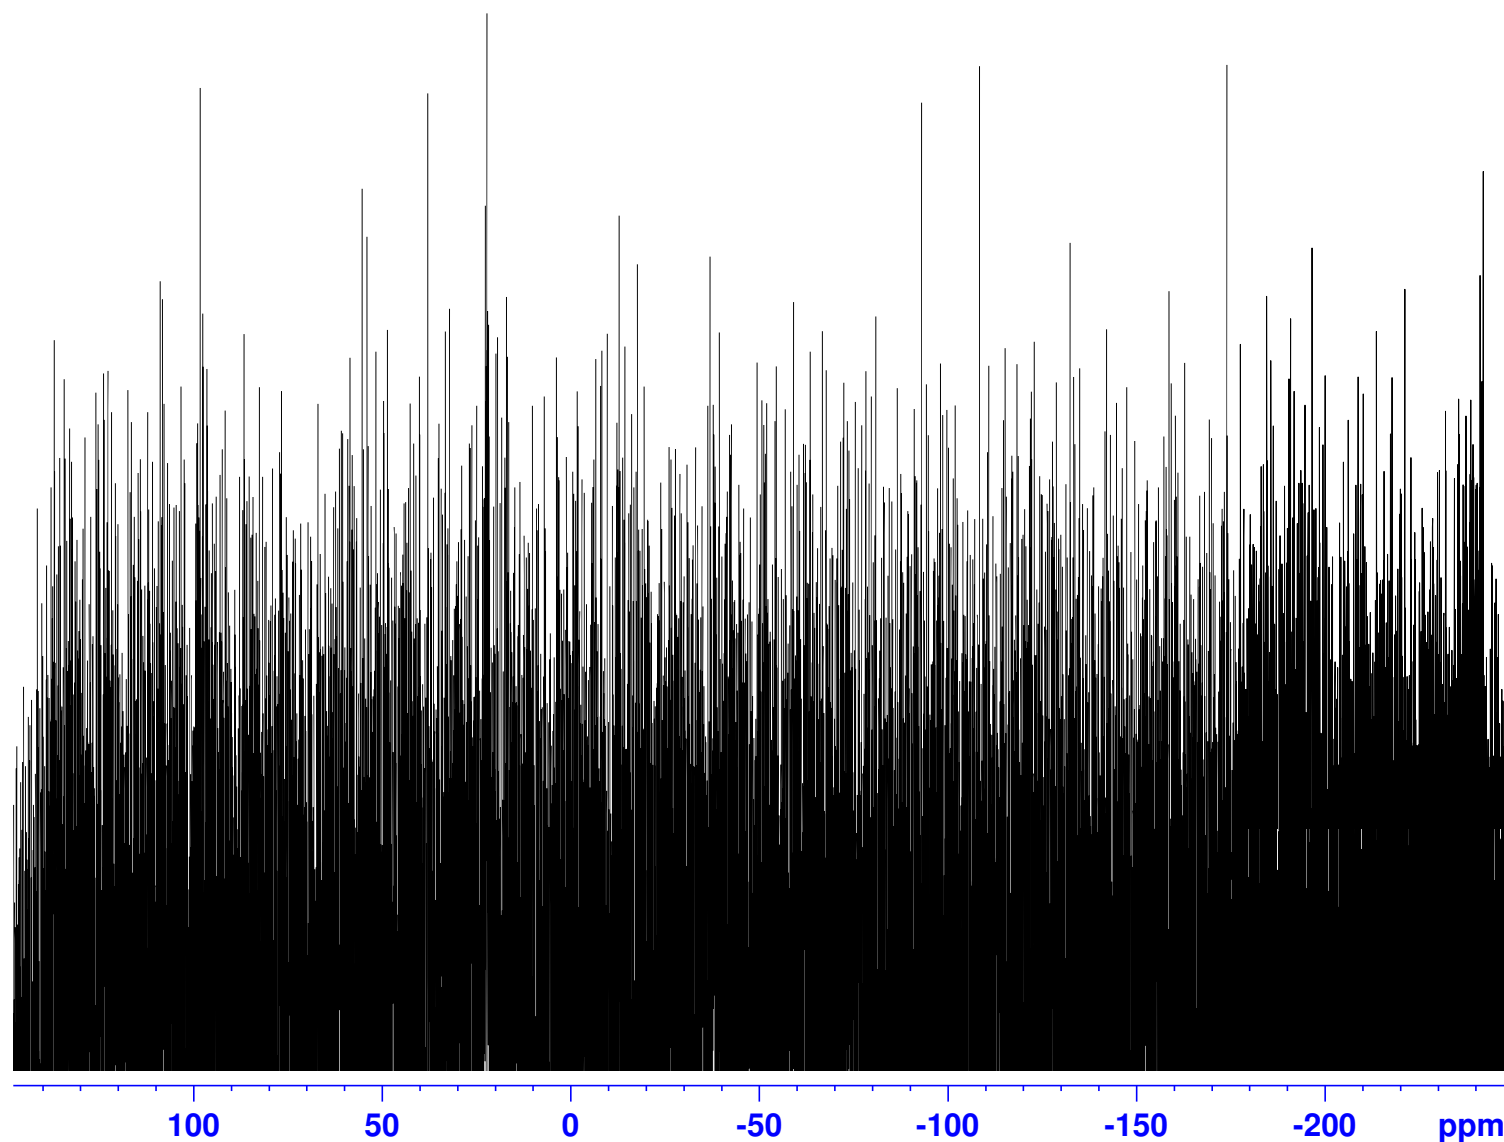

Current Data Parameters
NAME X_20181108
EXPNO 140
PROCNO 1

F2 - Acquisition Parameters
Date_ 20181109
Time 8.41 h
INSTRUM spect
PROBHD Z824801_0046 (
PULPROG zgpg30
TD 65536
SOLVENT CDC13
NS 16
DS 4
SWH 64102.562 Hz
FIDRES 1.956255 Hz
AQ 0.5111808 sec
RG 200.25
DW 7.800 usec
DE 6.50 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 162.0079729 MHz
NUC1 31P
P0 2.67 usec
P1 8.00 usec
PLW1 36.45100021 W
SFO2 400.2316009 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.23714000 W
PLW13 0.11928000 W

F2 - Processing parameters
SI 32768
SF 162.0160737 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

1.06
1.13
0.70
1.56
4.90
1.03
1.18
0.54
1.07
0.46
1.62
1.17
1.37
1.51
0.34
1.42
2.39
0.03
0.04
0.31
1.16
0.60
2.50
1.39
0.84
2.94
0.93
0.09
0.86
1.18
0.52
1.92
0.72
1.51
0.26
1.01
1.35
0.96
0.98
1.20
2.08
0.93
0.57
0.61
0.97