


BB07 - Pure Alkyne 1
P31CPD CDCl3 /opt/data Adv_Exp 22

28.99
24.24
21.71

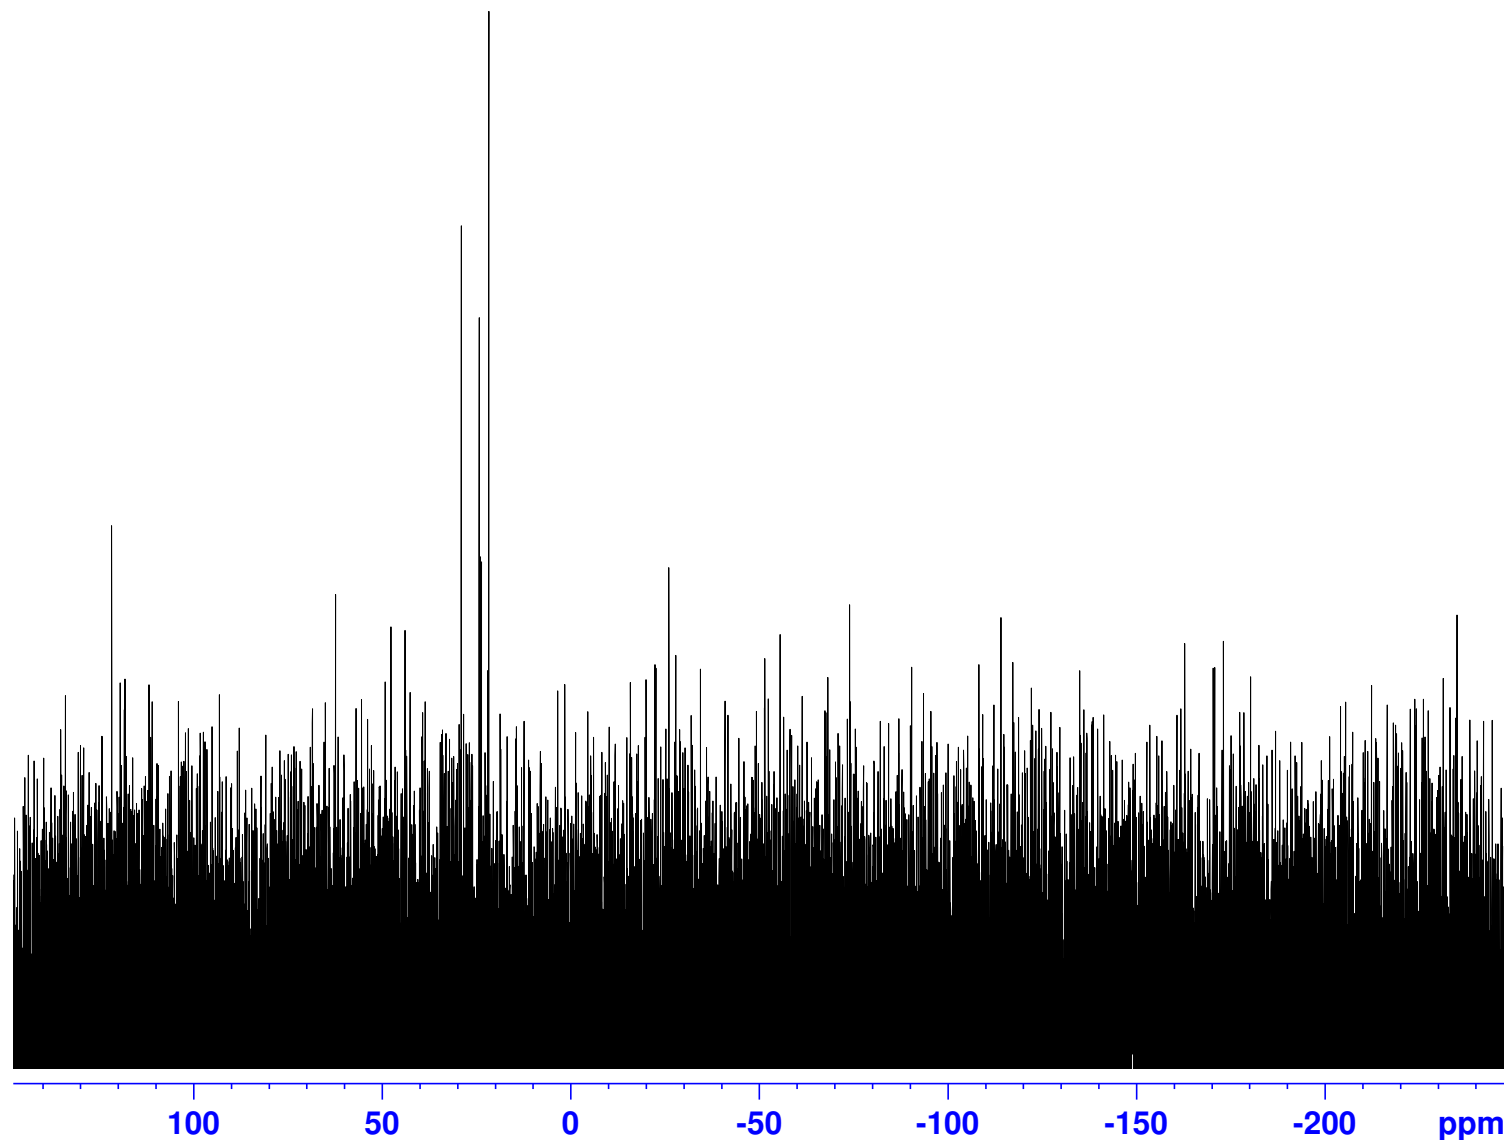

Current Data Parameters
NAME X_20181108
EXPNO 41
PROCNO 1

F2 - Acquisition Parameters
Date_ 20181108
Time 23.39 h
INSTRUM spect
PROBHD Z824801_0046 (
PULPROG zgpg30
TD 65536
SOLVENT CDCl3
NS 16
DS 4
SWH 64102.562 Hz
FIDRES 1.956255 Hz
AQ 0.5111808 sec
RG 200.25
DW 7.800 usec
DE 6.50 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 162.0079729 MHz
NUC1 31P
P0 2.67 usec
P1 8.00 usec
PLW1 36.45100021 W
SFO2 400.2316009 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.23714000 W
PLW13 0.11928000 W

F2 - Processing parameters
SI 32768
SF 162.0160737 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

0.52
0.55
1.26
1.12
0.19
2.01
8.37
8.46
1.28
0.47
0.24
3.05
0.99
1.25
0.85
2.48
0.53
1.02
1.79
0.51
0.37
0.77
1.57
0.70
1.06
1.80
1.58
0.50
0.06
1.00
0.47
1.44
0.31
0.68
1.56
0.31
1.99
1.52
0.24
1.92
1.04
1.00
0.44
1.57
1.44
1.88