


BB08 - Pure Alkyne 3
P31CPD CDC13 /opt/data Adv_Exp 23

24.19
21.99

Current Data Parameters
NAME X_20181108
EXPNO 51
PROCNO 1

F2 - Acquisition Parameters
Date_ 20181109
Time 0.02 h
INSTRUM spect
PROBHD Z824801_0046 (
PULPROG zgpg30
TD 65536
SOLVENT CDC13
NS 16
DS 4
SWH 64102.562 Hz
FIDRES 1.956255 Hz
AQ 0.5111808 sec
RG 200.25
DW 7.800 usec
DE 6.50 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 162.0079729 MHz
NUC1 31P
P0 2.67 usec
P1 8.00 usec
PLW1 36.45100021 W
SFO2 400.2316009 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.23714000 W
PLW13 0.11928000 W

F2 - Processing parameters
SI 32768
SF 162.0160737 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

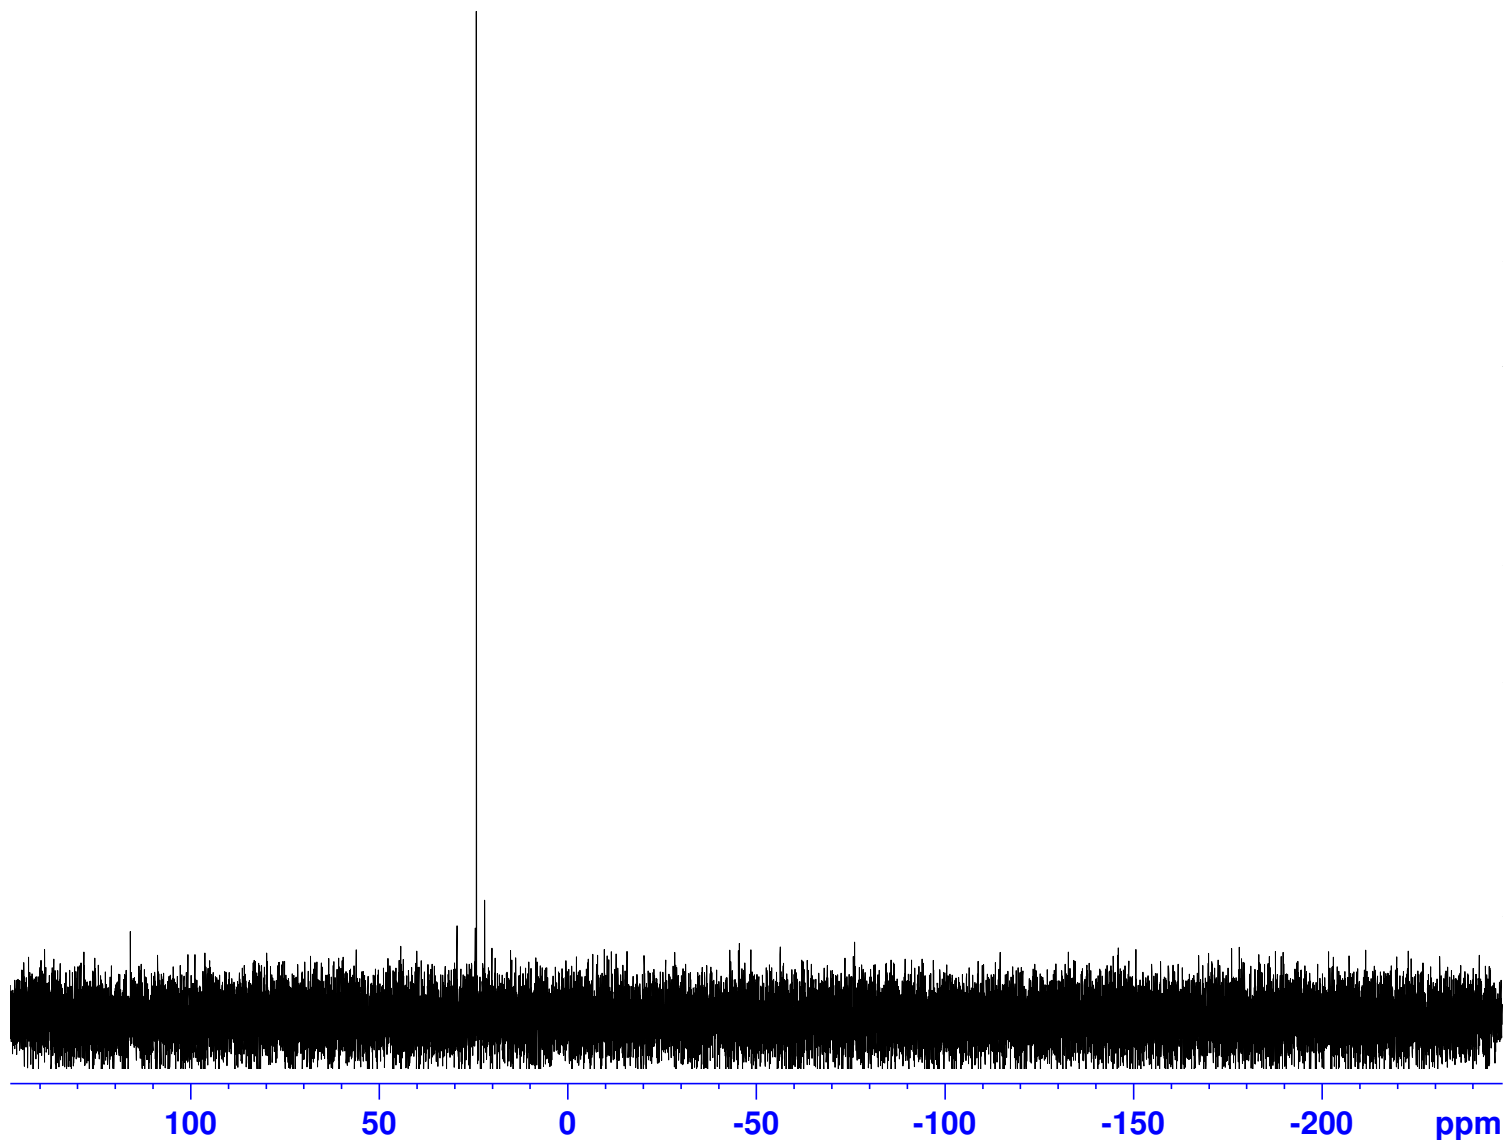

0.28 0.69 0.11 0.12 0.10 2.20 1.28 5.07 2.40 1.22 1.08 1.30 0.52 1.06 0.16 0.47 1.33 1.33 0.53 1.13 0.72 1.20 0.55 0.07 1.85 0.75 1.59 0.61 1.78 0.37 1.25 1.13 1.09 1.49 0.00 0.68 0.42 0.29 0.78 0.95 1.10 1.43 0.95 1.80 1.41 0.55