


AP 4 HP  
P31CPD CDC13 /opt/data Adv\_Exp 32

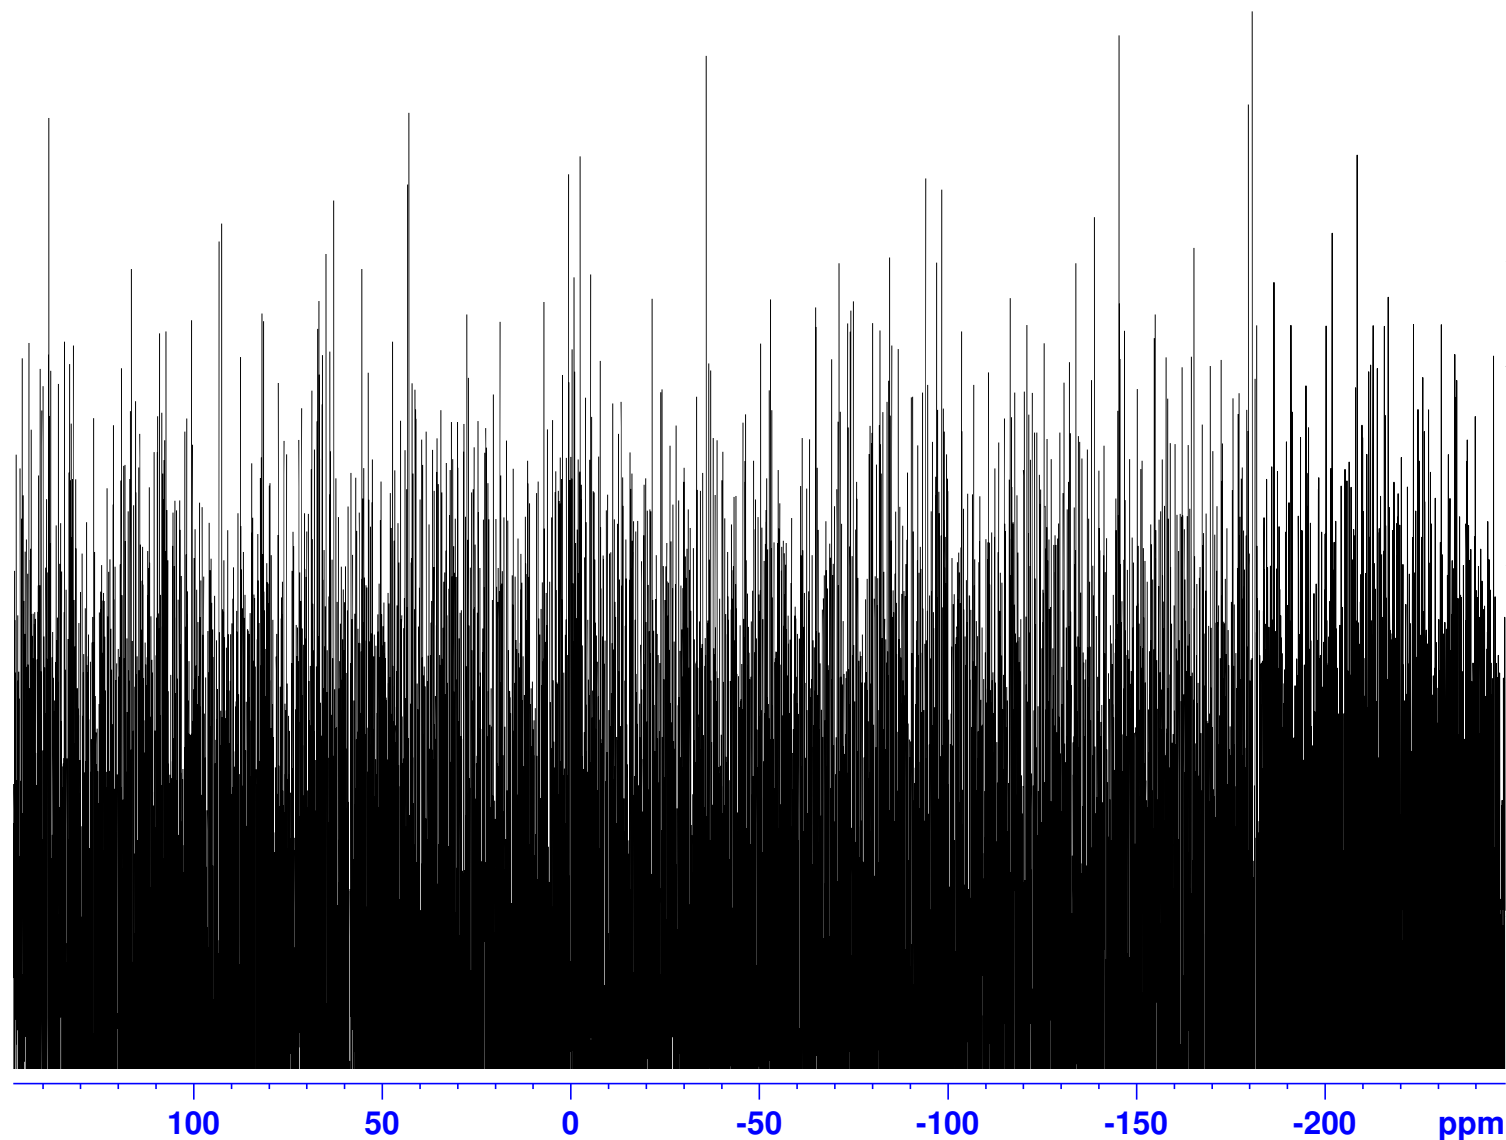

Current Data Parameters  
NAME X\_20181108  
EXPNO 72  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20181109  
Time 9.28 h  
INSTRUM spect  
PROBHD Z824801\_0046 (  
PULPROG zgpg30  
TD 65536  
SOLVENT CDC13  
NS 16  
DS 4  
SWH 64102.562 Hz  
FIDRES 1.956255 Hz  
AQ 0.5111808 sec  
RG 200.25  
DW 7.800 usec  
DE 6.50 usec  
TE 300.0 K  
D1 2.00000000 sec  
D11 0.03000000 sec  
TD0 1  
SFO1 162.0079729 MHz  
NUC1 31P  
P0 2.67 usec  
P1 8.00 usec  
PLW1 36.45100021 W  
SFO2 400.2316009 MHz  
NUC2 1H  
CPDPRG2 waltz16  
PCPD2 90.00 usec  
PLW2 20.00000000 W  
PLW12 0.23714000 W  
PLW13 0.11928000 W

F2 - Processing parameters  
SI 32768  
SF 162.0160737 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40

0.28  
0.75  
1.37  
1.97  
2.75  
0.08  
0.28  
1.74  
1.43  
1.71  
0.07  
0.80  
0.32  
0.36  
0.49  
0.75  
1.40  
0.67  
1.61  
0.64  
1.26  
1.51  
1.48  
2.10  
1.10  
2.14  
1.35  
1.09  
0.24  
1.44  
0.77  
0.15  
1.84  
2.19  
1.24  
1.97  
0.95  
0.74  
1.67  
1.97  
1.64  
0.05  
1.64  
1.25  
0.14  
1.29