


AP 1 PURE
P31CPD CDC13 /opt/data Adv_Exp 33

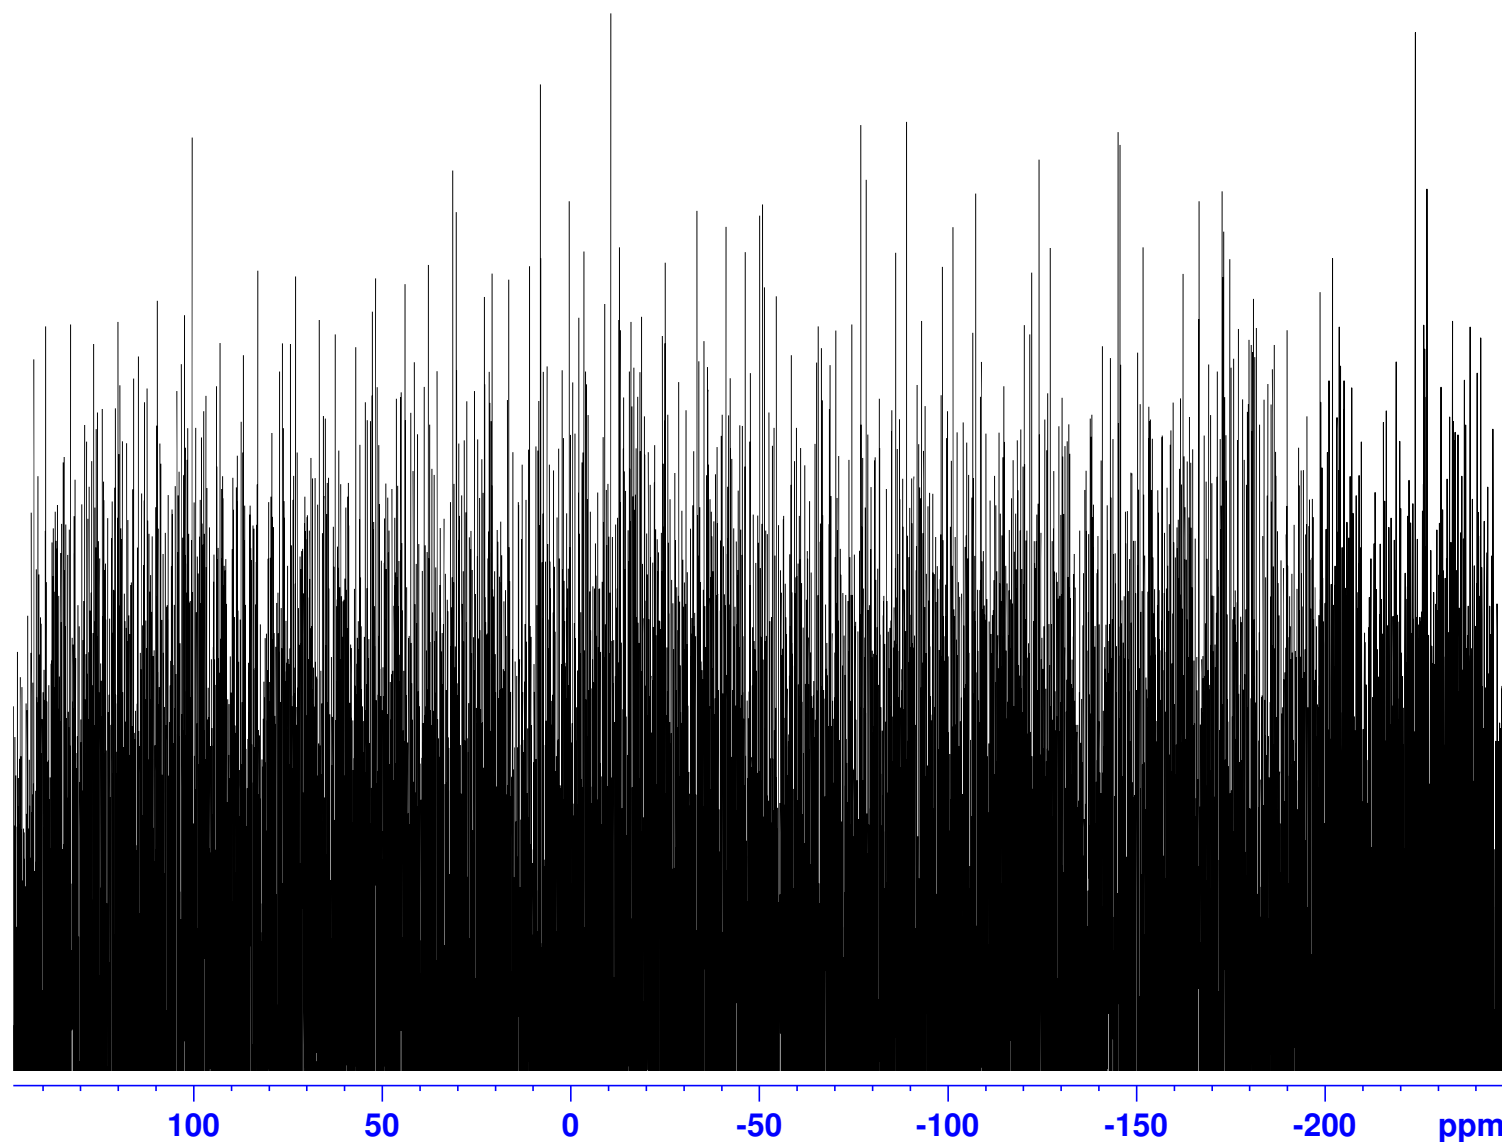

Current Data Parameters
NAME X_20181108
EXPNO 82
PROCNO 1

F2 - Acquisition Parameters
Date_ 20181109
Time 10.31 h
INSTRUM spect
PROBHD Z824801_0046 (
PULPROG zgpg30
TD 65536
SOLVENT CDC13
NS 16
DS 4
SWH 64102.562 Hz
FIDRES 1.956255 Hz
AQ 0.5111808 sec
RG 200.25
DW 7.800 usec
DE 6.50 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 162.0079729 MHz
NUC1 31P
P0 2.67 usec
P1 8.00 usec
PLW1 36.45100021 W
SFO2 400.2316009 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.23714000 W
PLW13 0.11928000 W

F2 - Processing parameters
SI 32768
SF 162.0160737 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

1.20
0.78
2.55
1.42
0.50
0.86
0.36
0.71
0.03
0.42
1.57
1.67
0.58
0.83
1.07
1.51
0.87
0.89
0.98
0.26
1.41
0.34
2.04
0.63
1.31
1.26
1.36
0.94
1.82
1.62
0.57
2.62
0.20
0.59
0.83
0.42
1.45
0.89
1.33
1.49
2.24
0.69
0.84
1.50
1.44
1.00