


Arefa boc1 sample yellow 1
PROTON.qm CDCl3 /opt/data Adv_Exp 38

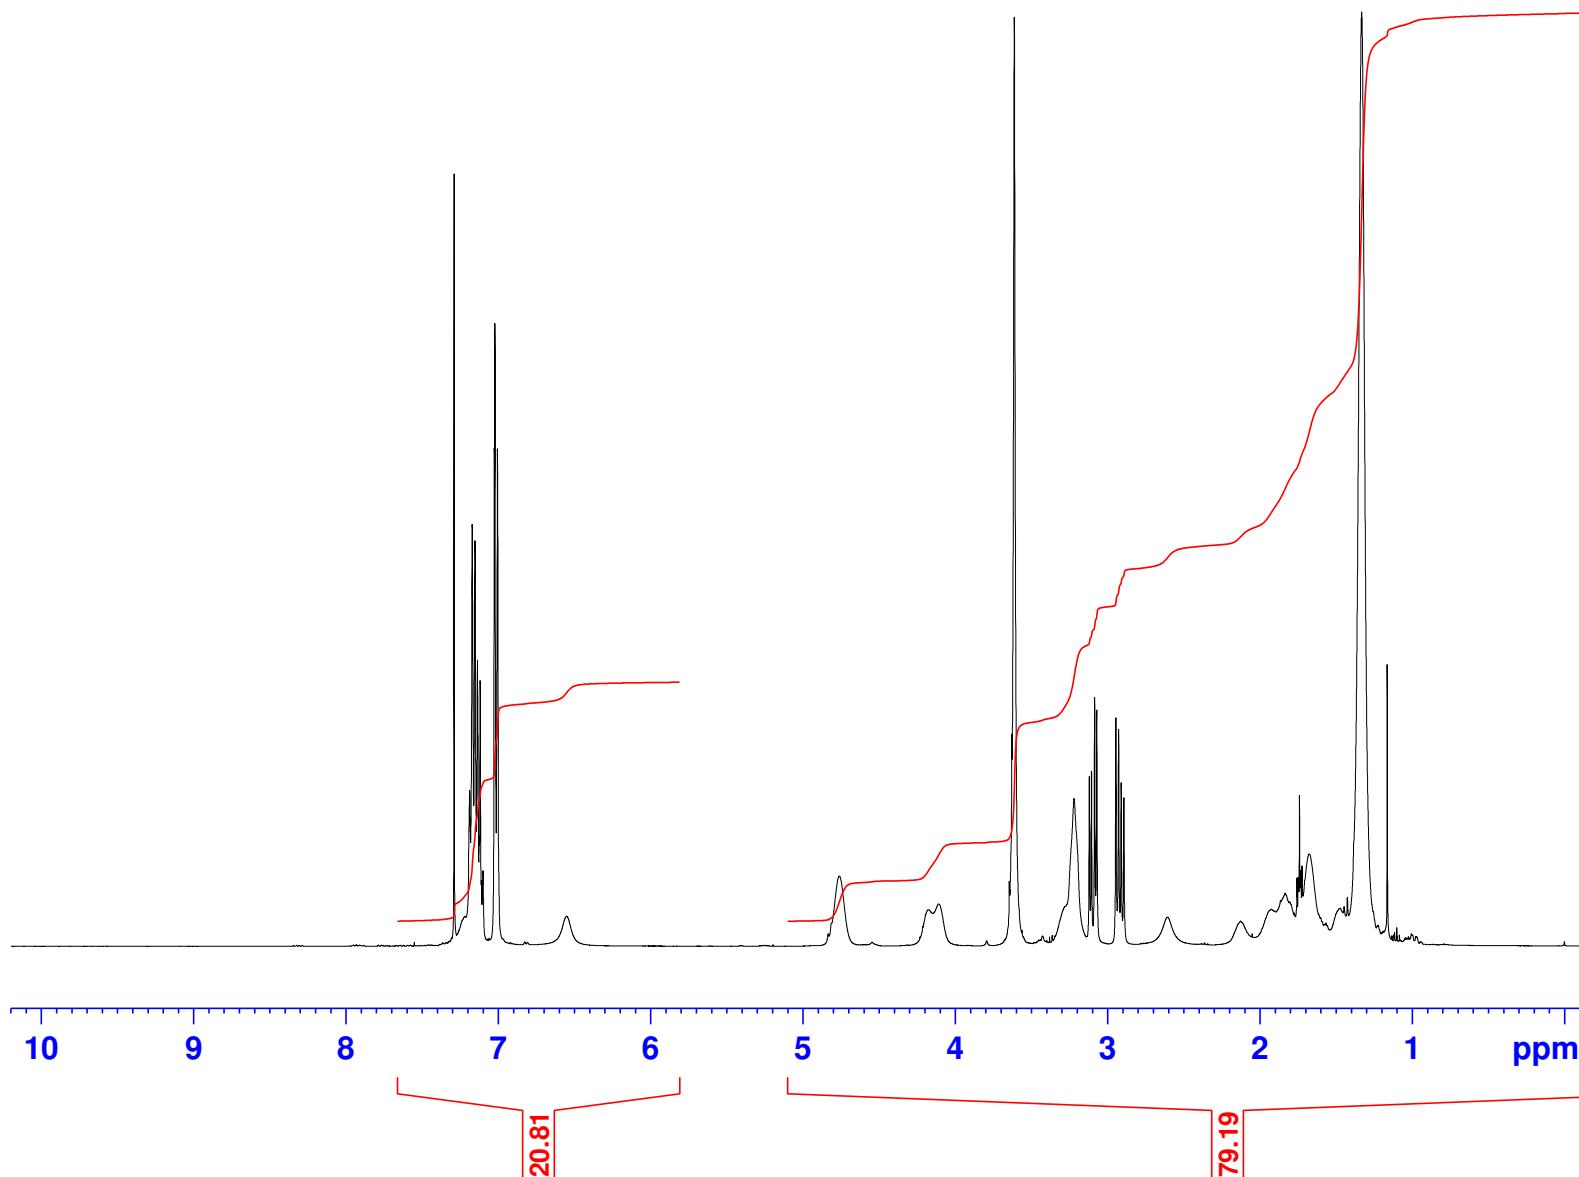

Current Data Parameters
NAME X_191029
EXPNO 320
PROCNO 1

F2 - Acquisition Parameters
Date_ 20191030
Time 5.58 h
INSTRUM aviii400
PROBHD Z108618_0305 (
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 16
DS 0
SWH 8223.685 Hz
FIDRES 0.250967 Hz
AQ 3.9845889 sec
RG 14.2
DW 60.800 usec
DE 16.89 usec
TE 300.0 K
D1 1.00000000 sec
TD0 1
SFO1 400.2024714 MHz
NUC1 1H
P0 4.07 usec
P1 12.20 usec
PLW1 19.95299911 W

F2 - Processing parameters
SI 65536
SF 400.1999969 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00