


NL2 - Meta Sub
P31CPD CDC13 /opt/data Adv_Exp 22

33.15
23.98

Current Data Parameters
NAME X_20190219
EXPNO 102
PROCNO 1

F2 - Acquisition Parameters
Date_ 20190219
Time 15.48 h
INSTRUM spect
PROBHD Z824801_0046 (
PULPROG zgpg30
TD 65536
SOLVENT CDC13
NS 16
DS 4
SWH 64102.562 Hz
FIDRES 1.956255 Hz
AQ 0.5111808 sec
RG 200.25
DW 7.800 usec
DE 6.50 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 162.0079729 MHz
NUC1 31P
P0 2.67 usec
P1 8.00 usec
PLW1 36.45100021 W
SFO2 400.2316009 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.23714000 W
PLW13 0.11928000 W

F2 - Processing parameters
SI 32768
SF 162.0160737 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

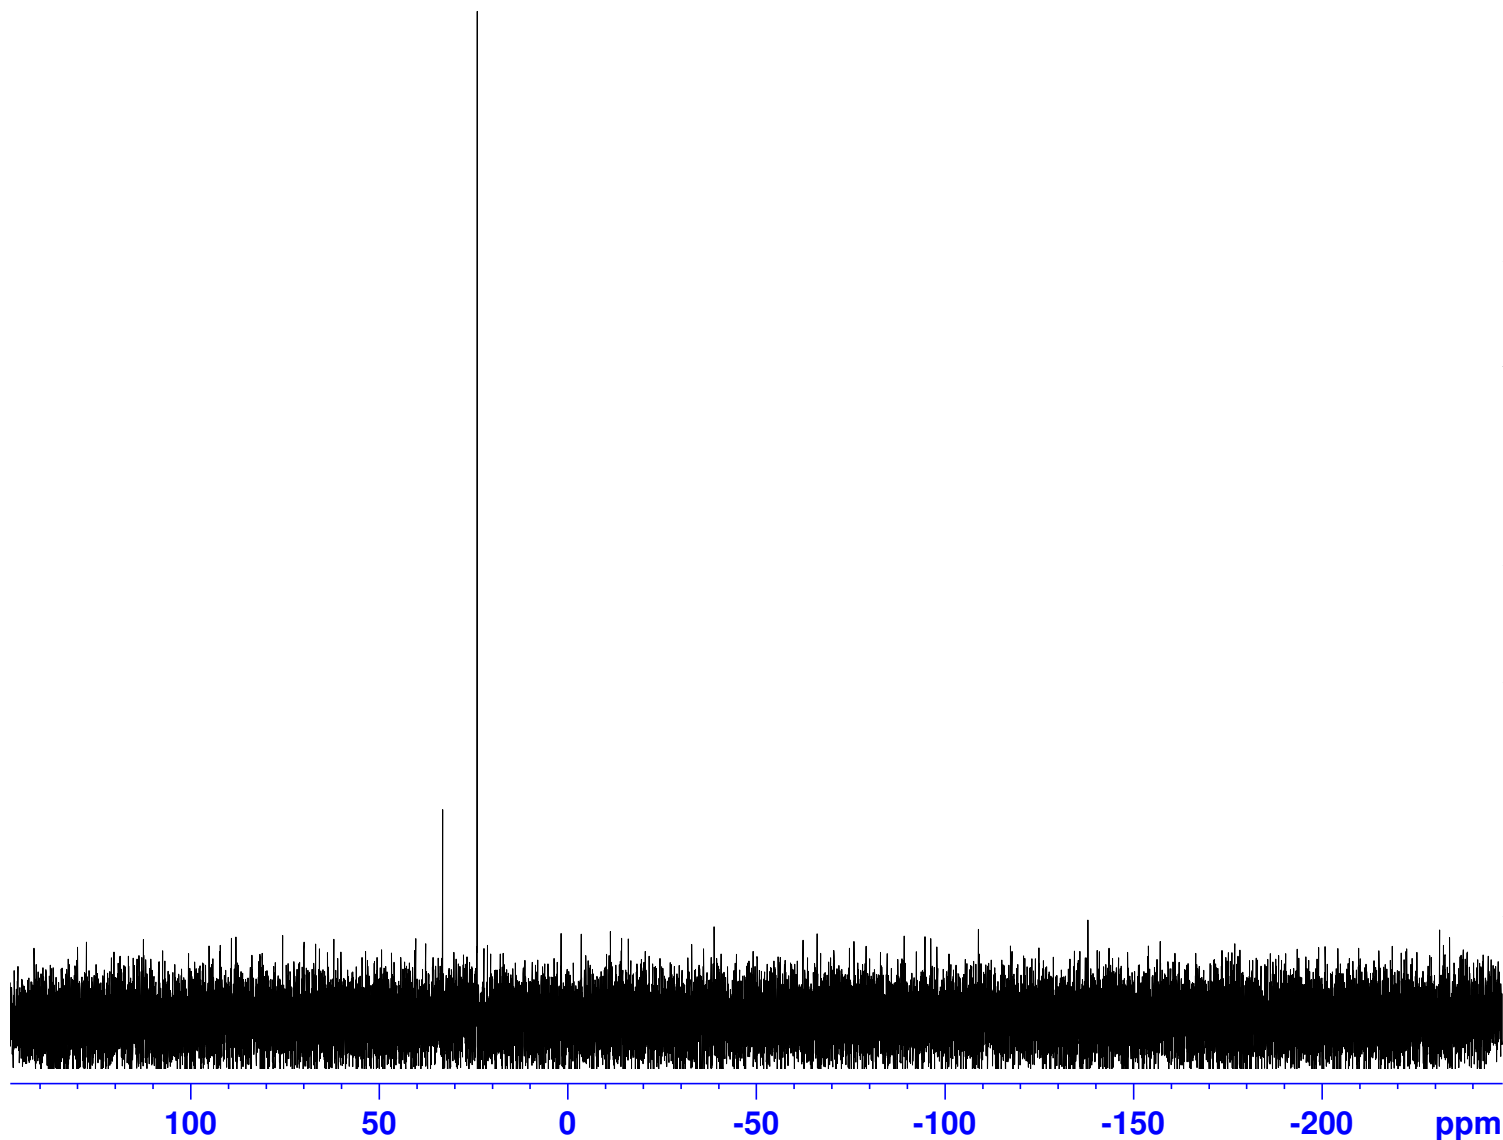

1.19
1.05
1.08
0.45
1.72
1.47
0.81
2.55
1.49
1.36
0.43
0.72
1.50
0.53
0.54
0.56
0.12
0.20
0.79
0.95
0.10
1.22
0.22
0.77
1.49
1.19
1.16
1.28
1.02
1.21
0.50
1.26
0.08
0.83
0.75
1.44
0.27
1.33
0.86
0.52
0.61
0.64
1.40
0.88
1.04
0.89