


NL1 PPH3
P31CPD CDC13 /opt/data Adv_Exp 21

23.22

Current Data Parameters
NAME X_20190219
EXPNO 112
PROCNO 1

F2 - Acquisition Parameters
Date_ 20190219
Time 15.25 h
INSTRUM spect
PROBHD Z824801_0046 (
PULPROG zgpg30
TD 65536
SOLVENT CDC13
NS 16
DS 4
SWH 64102.562 Hz
FIDRES 1.956255 Hz
AQ 0.5111808 sec
RG 200.25
DW 7.800 usec
DE 6.50 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 162.0079729 MHz
NUC1 31P
P0 2.67 usec
P1 8.00 usec
PLW1 36.45100021 W
SFO2 400.2316009 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.23714000 W
PLW13 0.11928000 W

F2 - Processing parameters
SI 32768
SF 162.0160737 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

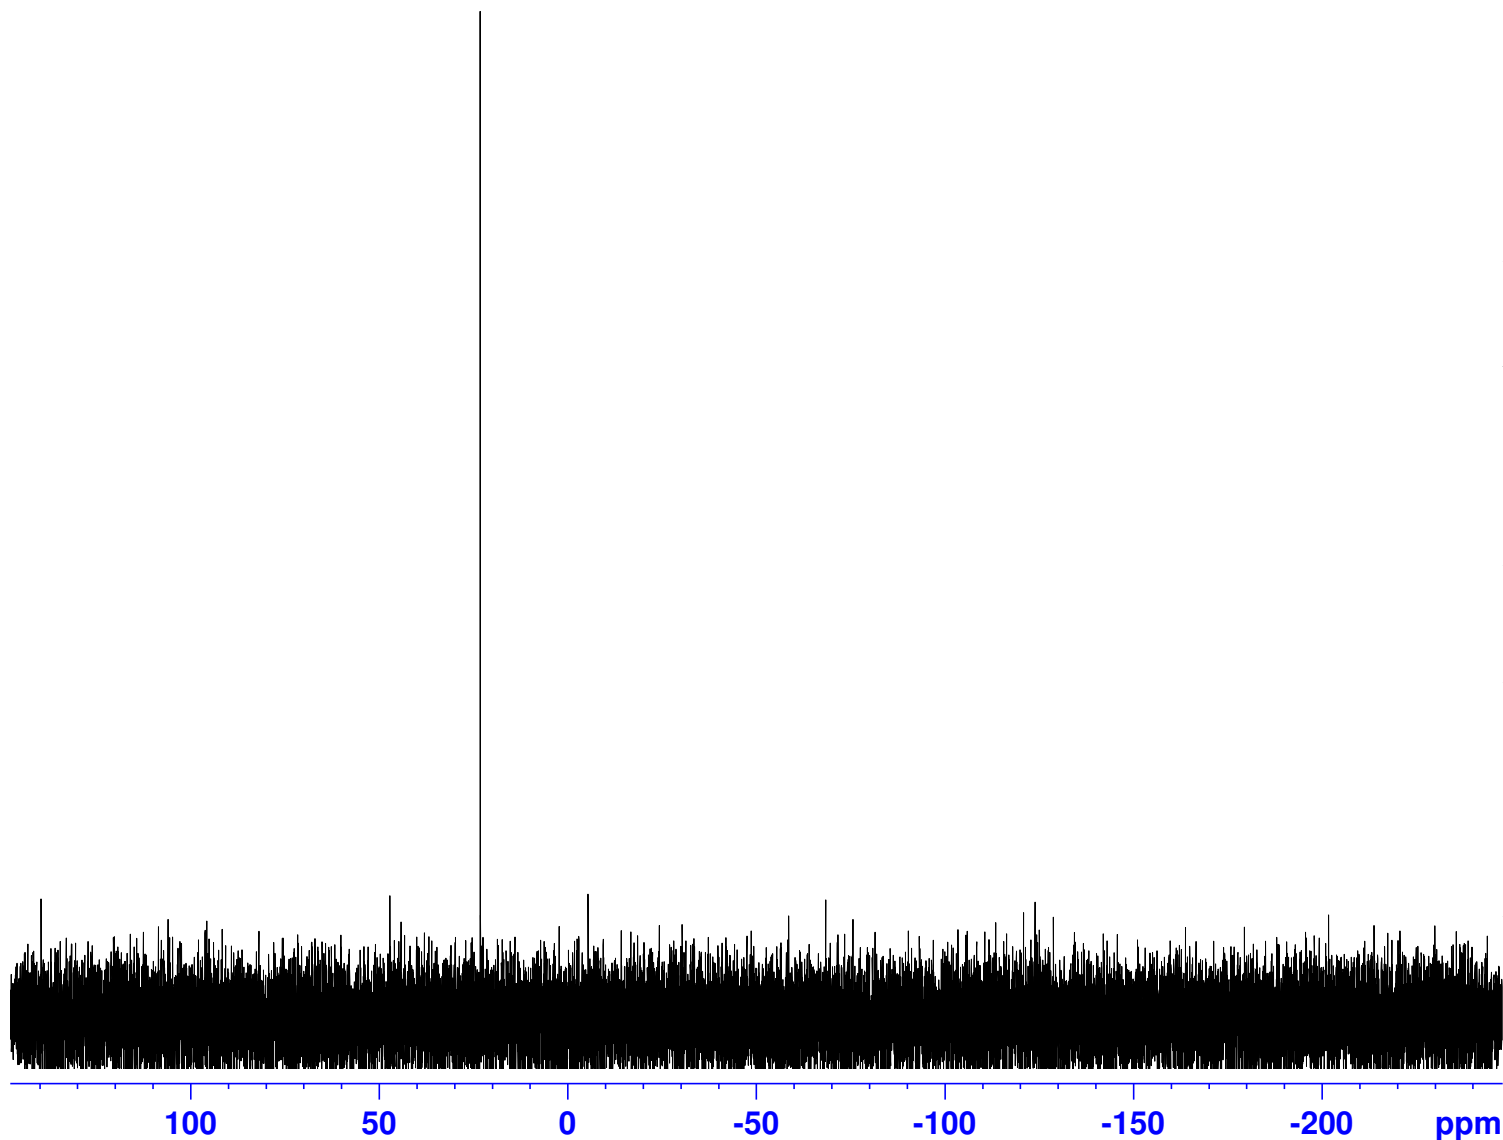

1.20
1.23
0.37
3.05
0.87
0.54
2.15
0.38
0.03
0.54
0.51
1.54
0.91
1.27
0.67
1.55
0.26
1.84
0.99
0.84
1.28
1.07
0.83
1.07
0.92
0.85
1.21
2.08
1.86
0.61
1.16
3.71
1.21
0.72
0.04
0.77
1.63
1.65
1.10
1.12
2.04
0.18
1.26
0.04
0.81
1.20