


tkapoor compund 2  
P31CPD CDC13 /opt/data Adv\_Exp 36

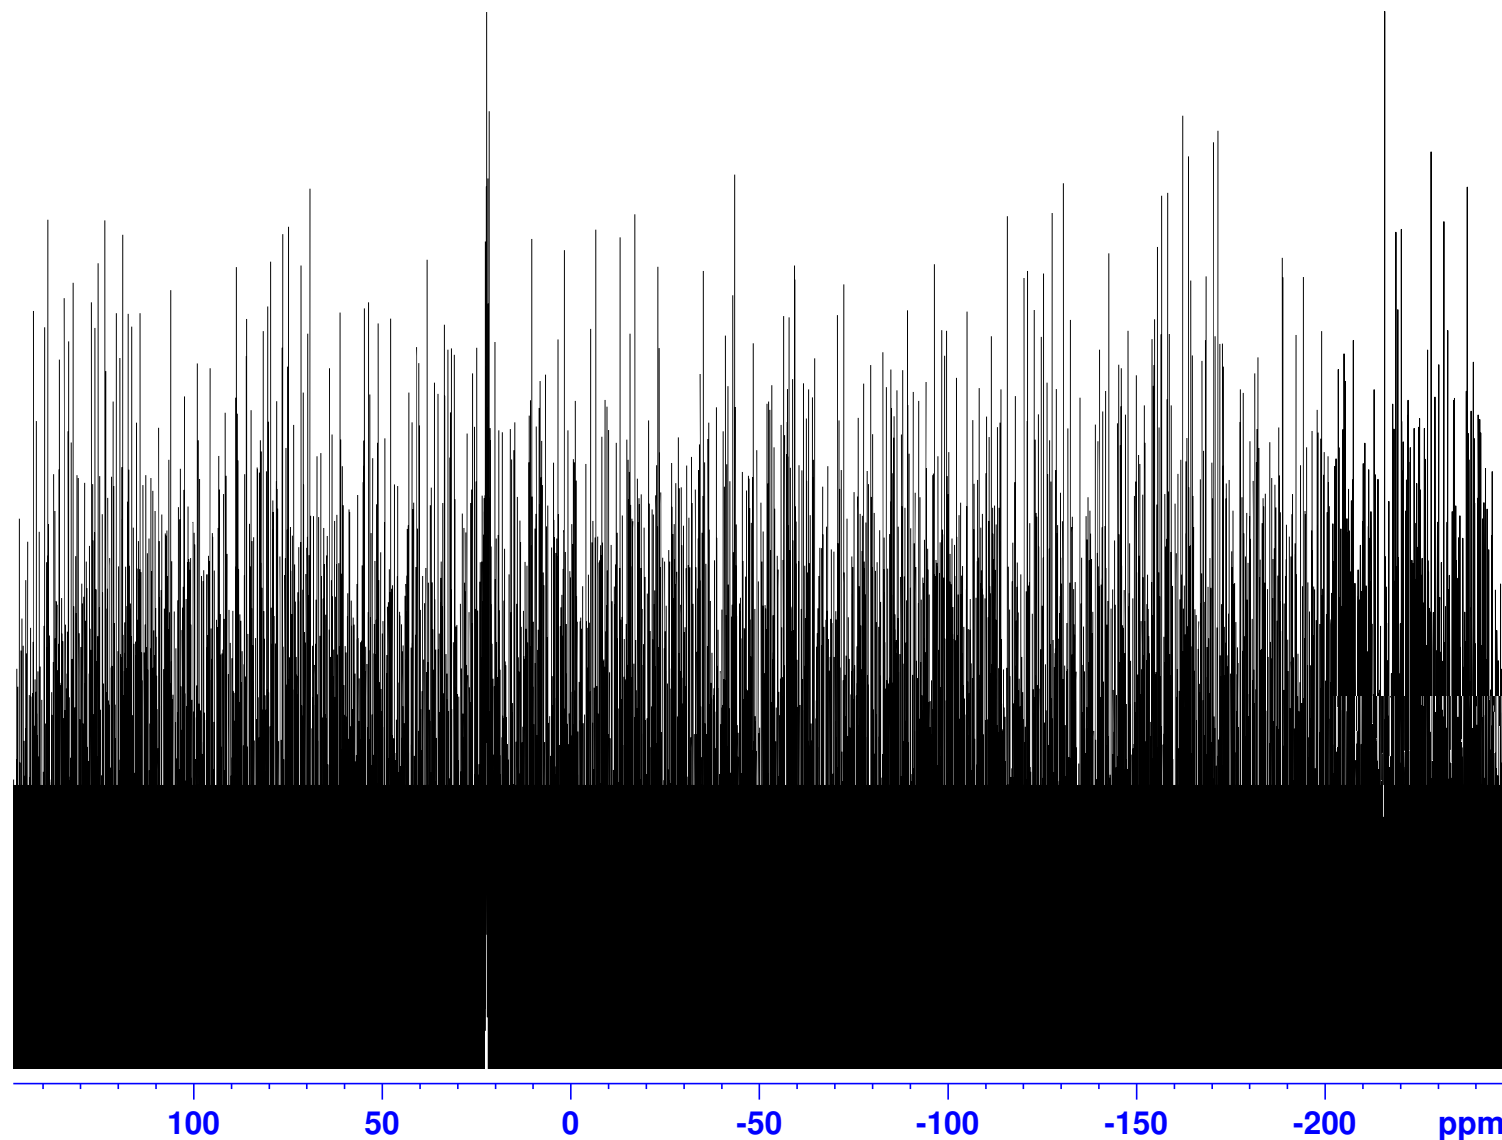

Current Data Parameters  
NAME X\_20190219  
EXPNO 152  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20190219  
Time 14.39 h  
INSTRUM spect  
PROBHD Z824801\_0046 (  
PULPROG zgpg30  
TD 65536  
SOLVENT CDC13  
NS 16  
DS 4  
SWH 64102.562 Hz  
FIDRES 1.956255 Hz  
AQ 0.5111808 sec  
RG 200.25  
DW 7.800 usec  
DE 6.50 usec  
TE 300.0 K  
D1 2.00000000 sec  
D11 0.03000000 sec  
TD0 1  
SFO1 162.0079729 MHz  
NUC1 31P  
P0 2.67 usec  
P1 8.00 usec  
PLW1 36.45100021 W  
SFO2 400.2316009 MHz  
NUC2 1H  
CPDPRG2 waltz16  
PCPD2 90.00 usec  
PLW2 20.00000000 W  
PLW12 0.23714000 W  
PLW13 0.11928000 W

F2 - Processing parameters  
SI 32768  
SF 162.0160737 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40

0.64  
0.18  
0.38  
2.04  
0.02  
0.91  
1.83  
0.24  
6.73  
1.30  
1.85  
0.75  
2.42  
1.59  
1.20  
1.48  
0.31  
0.78  
1.30  
0.78  
1.24  
0.49  
2.02  
0.93  
0.40  
0.01  
0.73  
0.53  
1.93  
0.87  
1.70  
0.50  
0.27  
1.75  
0.99  
1.12  
1.27  
1.11  
1.16  
0.13  
1.15  
1.21  
1.50  
1.07  
0.83  
1.67