


Suliman Comp 1
P31CPD CDC13 /opt/data Adv_Exp 52

23.24

Current Data Parameters
NAME X_20190219
EXPNO 302
PROCNO 1

F2 - Acquisition Parameters
Date_ 20190219
Time 20.25 h
INSTRUM spect
PROBHD Z824801_0046 (
PULPROG zgpg30
TD 65536
SOLVENT CDC13
NS 16
DS 4
SWH 64102.562 Hz
FIDRES 1.956255 Hz
AQ 0.5111808 sec
RG 200.25
DW 7.800 usec
DE 6.50 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 162.0079729 MHz
NUC1 31P
P0 2.67 usec
P1 8.00 usec
PLW1 36.45100021 W
SFO2 400.2316009 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.23714000 W
PLW13 0.11928000 W

F2 - Processing parameters
SI 32768
SF 162.0160737 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

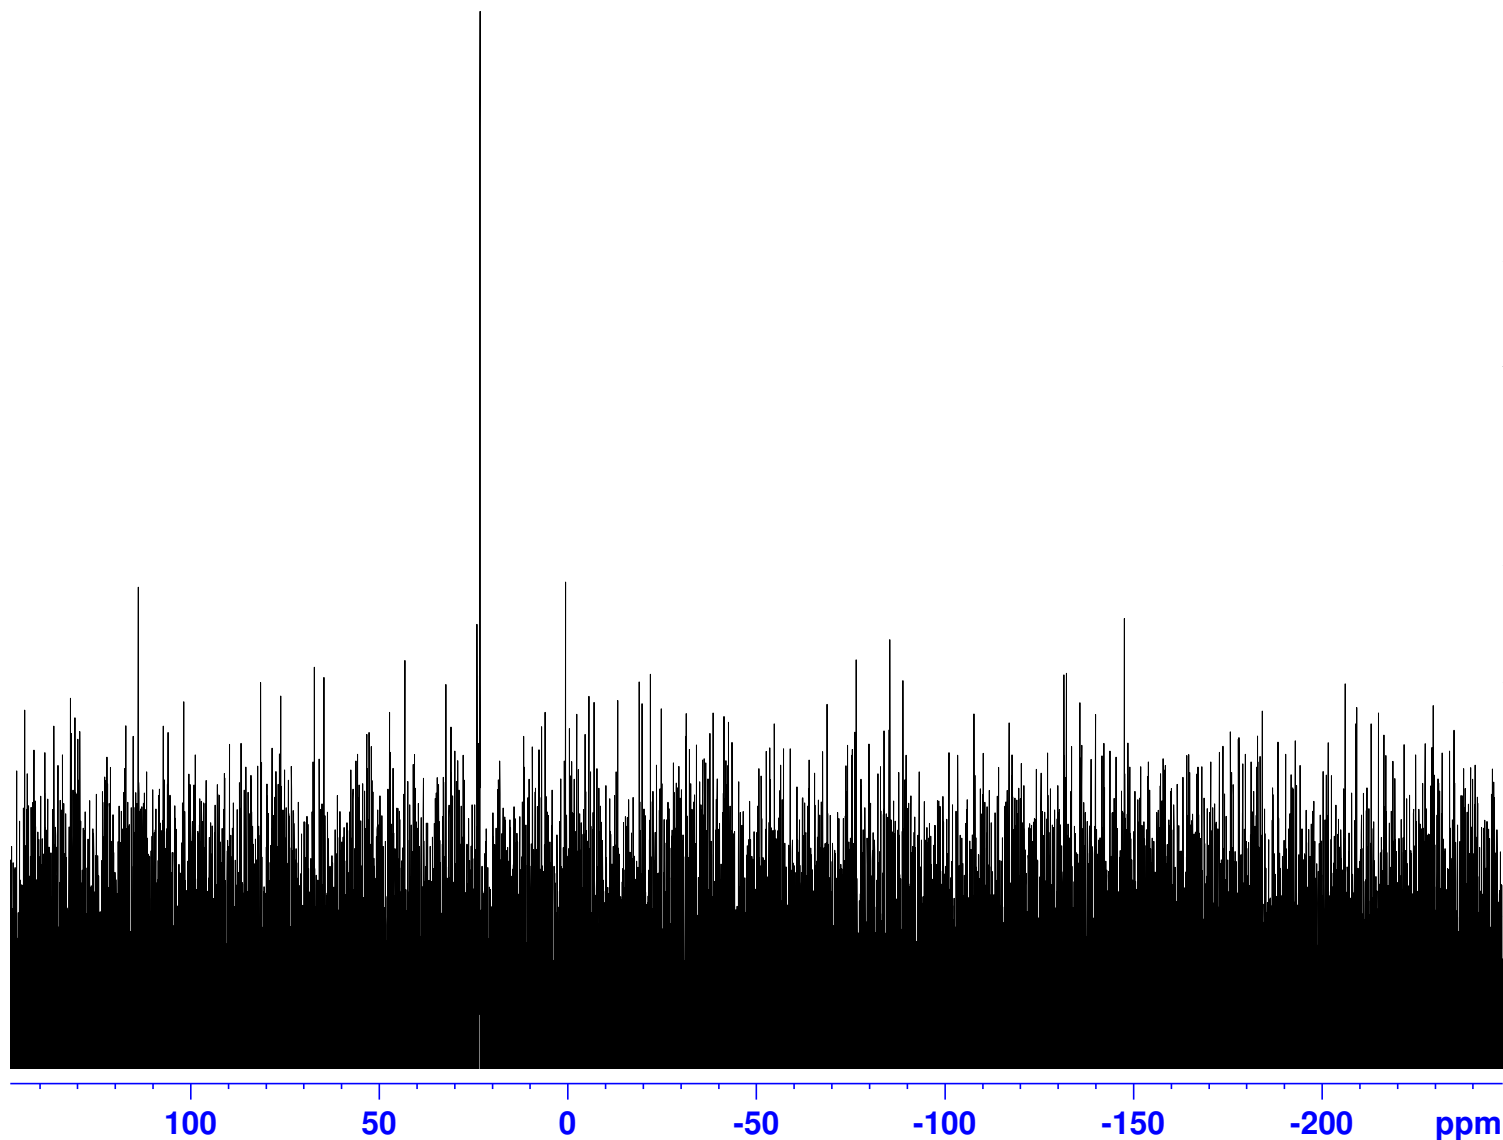

1.07 1.64 3.18 0.59 1.51 1.78 8.57 0.61 1.90 0.69 0.52 1.64 2.88 0.50 2.06 0.90 0.76 0.26 0.10 0.12 2.49 0.02 0.52 0.45 2.67 0.30 1.19 1.23 1.02 1.10 0.19 0.47 1.12 0.86 1.10 0.36 0.28 0.47 1.06 2.25 0.93 0.81 0.52 1.05 0.68 1.24