


Suliman Comp 4
P31CPD CDC13 /opt/data Adv_Exp 53

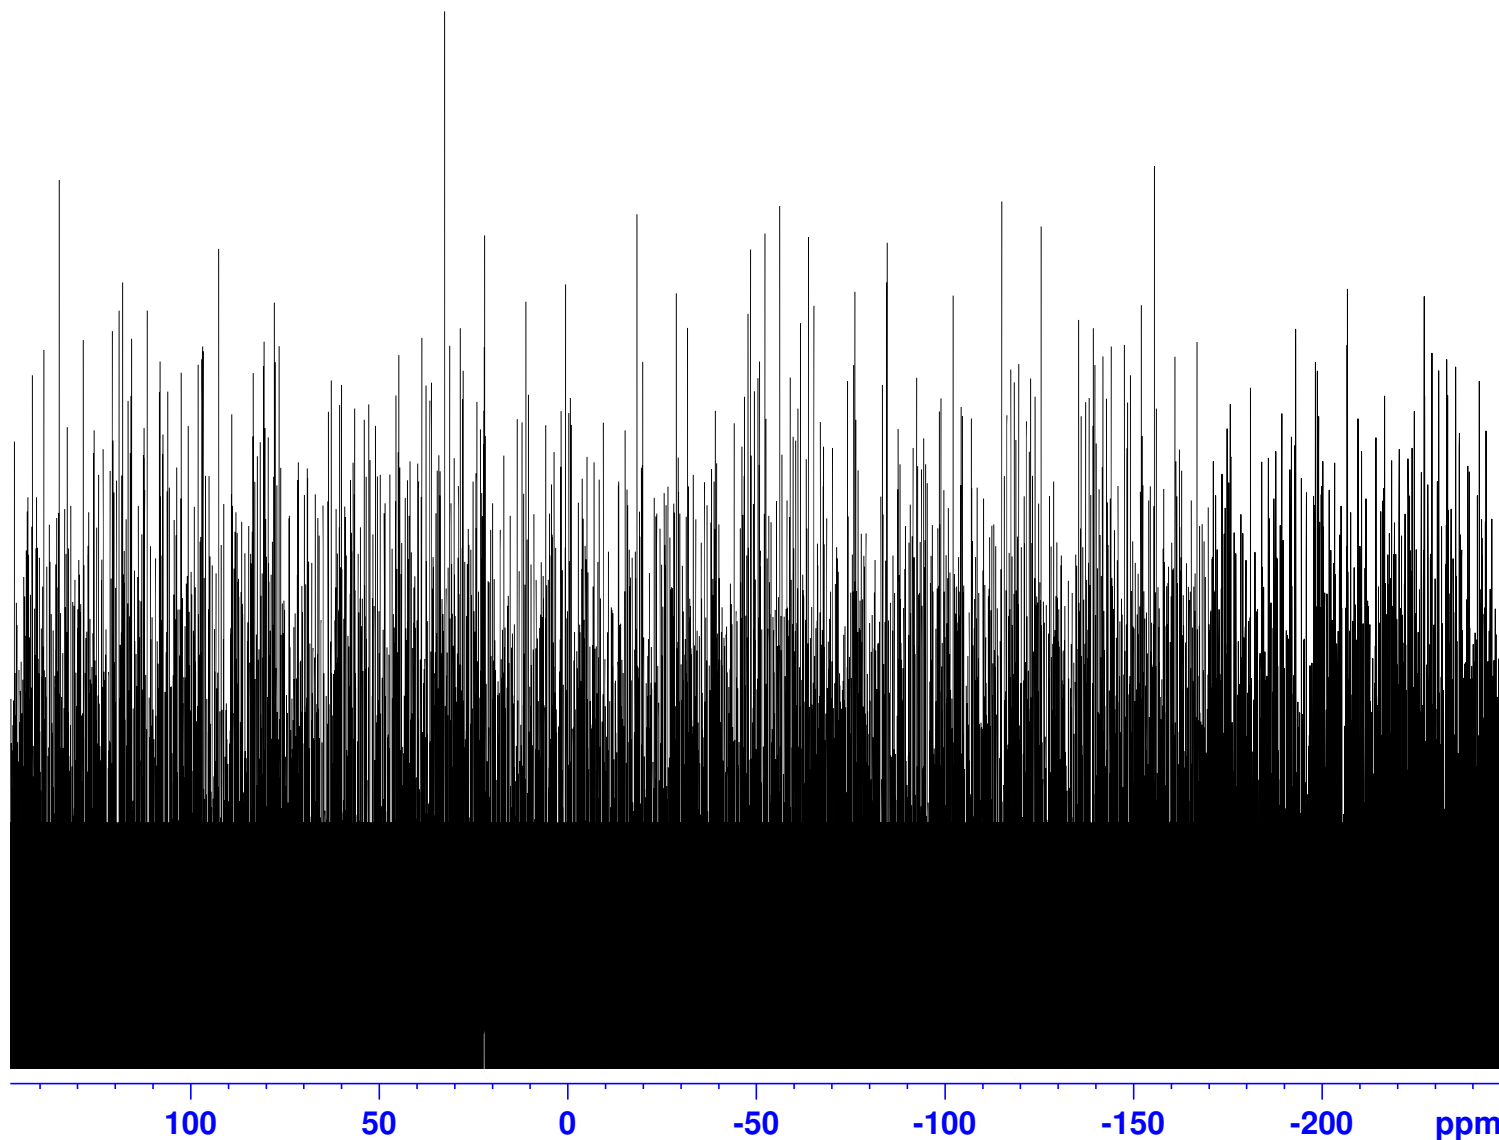

Current Data Parameters
NAME X_20190219
EXPNO 312
PROCNO 1

F2 - Acquisition Parameters
Date_ 20190219
Time 20.48 h
INSTRUM spect
PROBHD Z824801_0046 (
PULPROG zgpg30
TD 65536
SOLVENT CDC13
NS 16
DS 4
SWH 64102.562 Hz
FIDRES 1.956255 Hz
AQ 0.5111808 sec
RG 200.25
DW 7.800 usec
DE 6.50 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 162.0079729 MHz
NUC1 31P
P0 2.67 usec
P1 8.00 usec
PLW1 36.45100021 W
SFO2 400.2316009 MHz
NUC2 1H
CPDPRG2 waltz16
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.23714000 W
PLW13 0.11928000 W

F2 - Processing parameters
SI 32768
SF 162.0160737 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

0.22 0.29 1.80 1.43 0.65 0.23 0.96 1.21 0.12 1.33 2.24 0.05 1.38 1.05 1.81 0.45 0.83 1.86 1.16 0.82 1.92 3.20 0.84 0.90 0.77 0.98 0.85 0.15 0.32 1.06 1.46 1.21 1.51 0.01 0.66 2.14 1.32 0.61 0.98 3.39 0.64 0.82 1.59 1.65 0.96