


marouf comp 1
P31CPD CDCl3 /opt/data Adv_Exp 54

Current Data Parameters
NAME X_20190219
EXPNO 322
PROCNO 1

F2 - Acquisition Parameters
Date_ 20190219
Time 21.11 h
INSTRUM spect
PROBHD Z824801_0046 (
PULPROG zgpg30
TD 65536
SOLVENT CDCl3
NS 16
DS 4
SWH 64102.562 Hz
FIDRES 1.956255 Hz
AQ 0.5111808 sec
RG 200.25
DW 7.800 usec
DE 6.50 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 162.0079729 MHz
NUC1 31P
P0 2.67 usec
P1 8.00 usec
PLW1 36.45100021 W
SFO2 400.2316009 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.23714000 W
PLW13 0.11928000 W

F2 - Processing parameters
SI 32768
SF 162.0160737 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

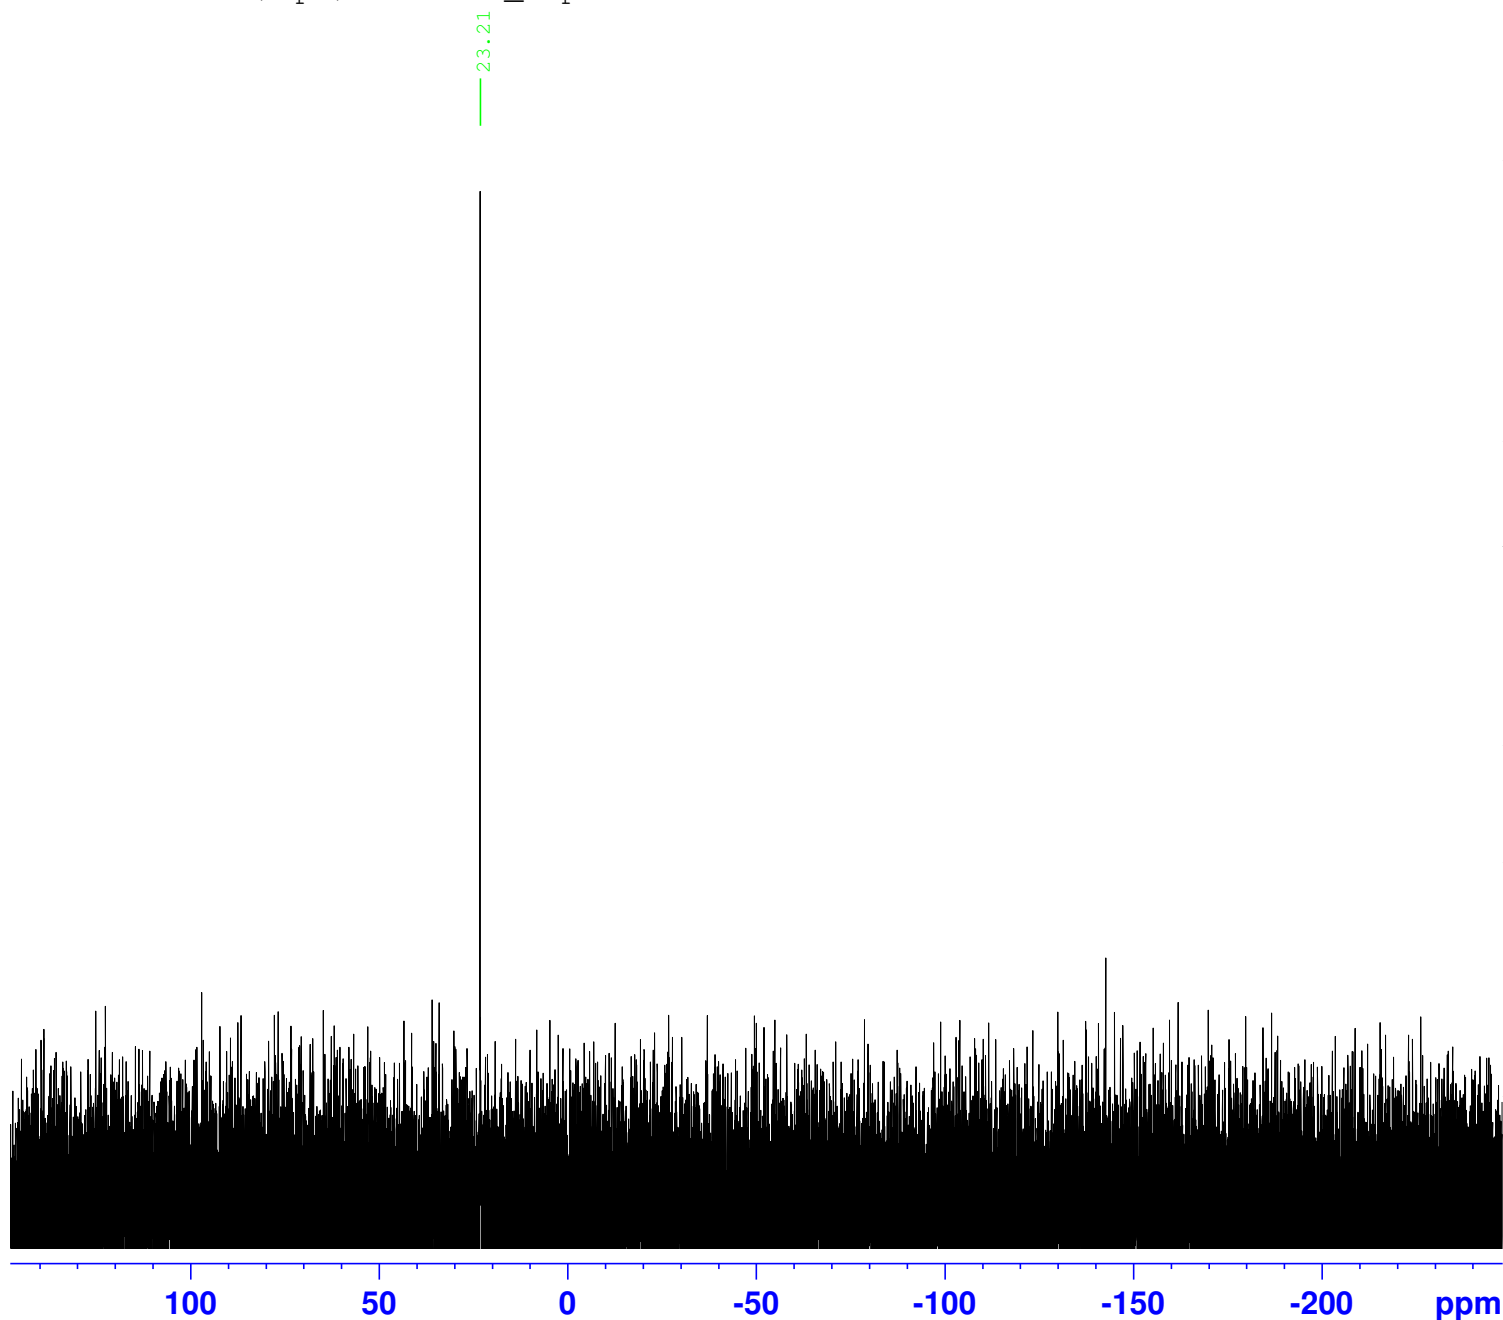

0.65
1.17
0.71
0.52
0.27
1.59
0.84
2.02
0.99
0.50
0.71
3.09
1.12
1.05
2.28
2.55
2.14
0.02
1.89
0.54
0.65
0.10
0.23
2.55
2.79
0.38
0.19
2.20
0.08
0.87
0.64
0.48
0.50
1.04
1.21
2.76
0.98
0.63
1.78
0.02
0.55
0.10
2.32
1.32
1.18
0.67