


tkapoor compound 2
P31CPD CDC13 /opt/data Adv_Exp 36

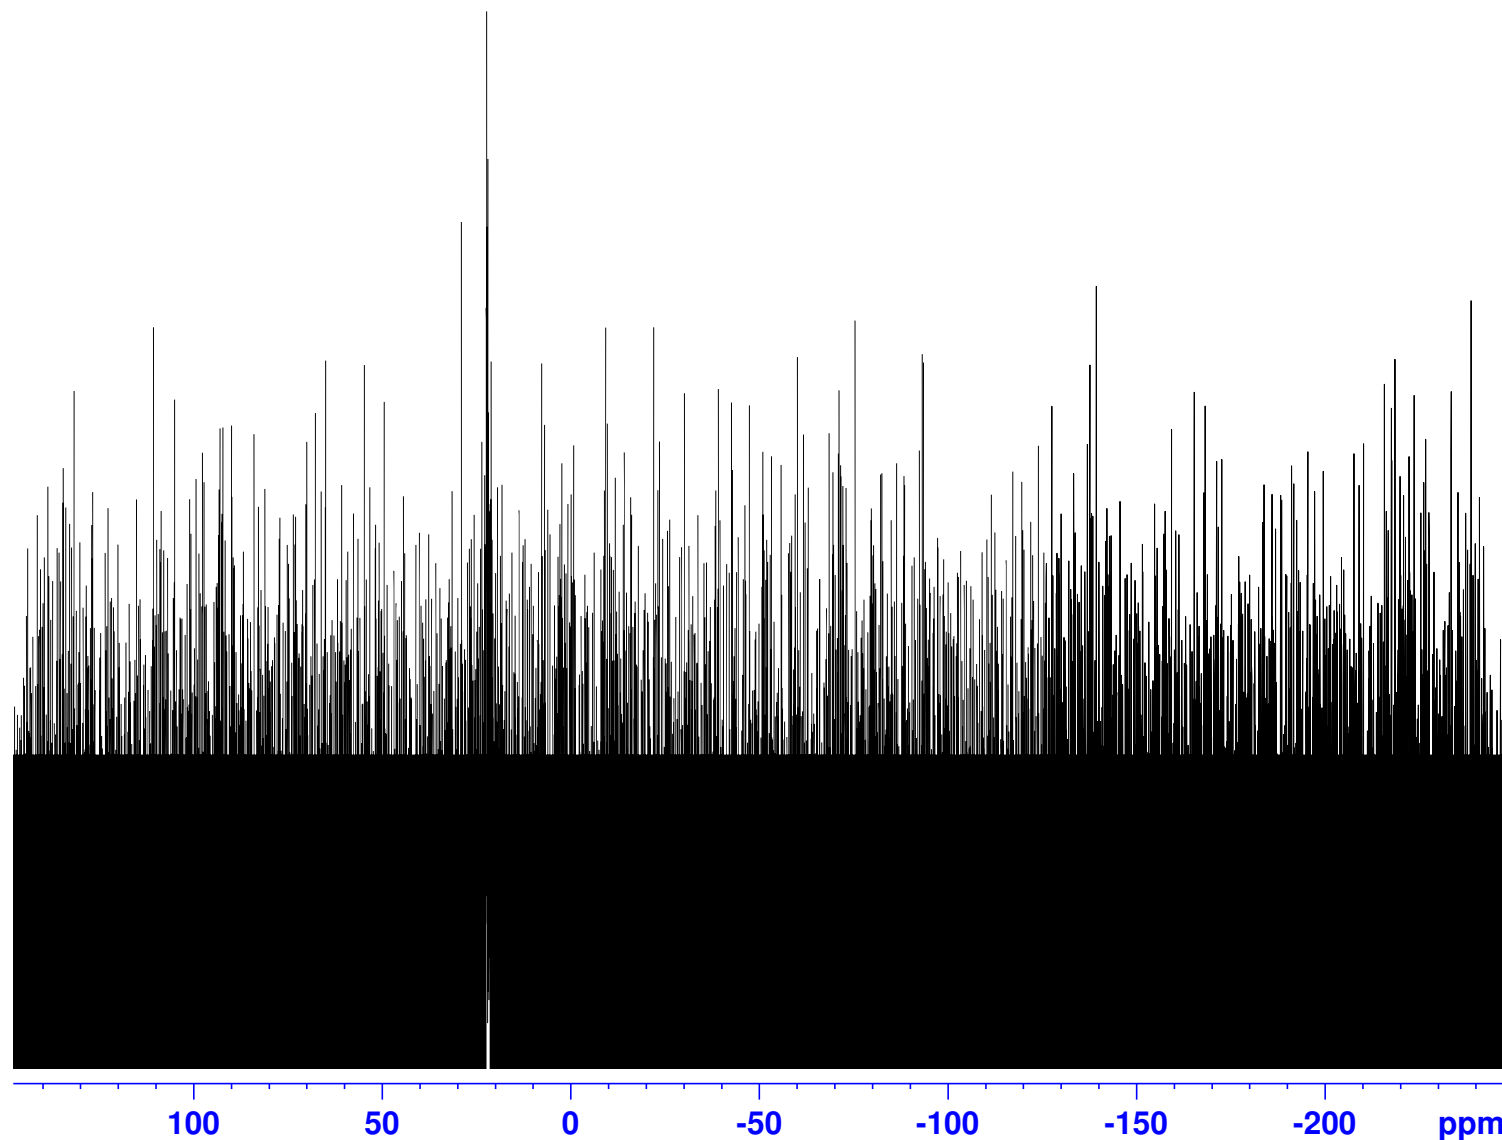

Current Data Parameters
NAME X_20190219
EXPNO 342
PROCNO 1

F2 - Acquisition Parameters
Date_ 20190219
Time 22.01 h
INSTRUM spect
PROBHD Z824801_0046 (
PULPROG zgpg30
TD 65536
SOLVENT CDCl3
NS 16
DS 4
SWH 64102.562 Hz
FIDRES 1.956255 Hz
AQ 0.5111808 sec
RG 200.25
DW 7.800 usec
DE 6.50 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 162.0079729 MHz
NUC1 31P
P0 2.67 usec
P1 8.00 usec
PLW1 36.45100021 W
SFO2 400.2316009 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.23714000 W
PLW13 0.11928000 W

F2 - Processing parameters
SI 32768
SF 162.0160737 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

0.28
1.31
0.57
1.14
3.37
2.73
1.17
0.66
1.90
0.40
1.12
0.95
0.05
1.17
0.80
0.38
0.10
0.09
0.79
1.35
0.78
0.29
1.53
1.16
0.19
1.15
0.59
0.28
0.81
0.43
0.54
0.45
0.83
1.20
0.95
0.88
1.10
2.95
1.25
0.69
1.32
0.35
1.92
0.59
2.45
0.33