


Suliman Comp 4
P31CPD CDC13 /opt/data Adv_Exp 10

Current Data Parameters
NAME X_20190219
EXPNO 54
PROCNO 1

F2 - Acquisition Parameters
Date_ 20190219
Time 15.02 h
INSTRUM spect
PROBHD Z824801_0046 (
PULPROG zgpg30
TD 65536
SOLVENT CDC13
NS 16
DS 4
SWH 64102.562 Hz
FIDRES 1.956255 Hz
AQ 0.5111808 sec
RG 200.25
DW 7.800 usec
DE 6.50 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 162.0079729 MHz
NUC1 31P
P0 2.67 usec
P1 8.00 usec
PLW1 36.45100021 W
SFO2 400.2316009 MHz
NUC2 1H
CPDPRG2 waltz16
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.23714000 W
PLW13 0.11928000 W

F2 - Processing parameters
SI 32768
SF 162.0160737 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

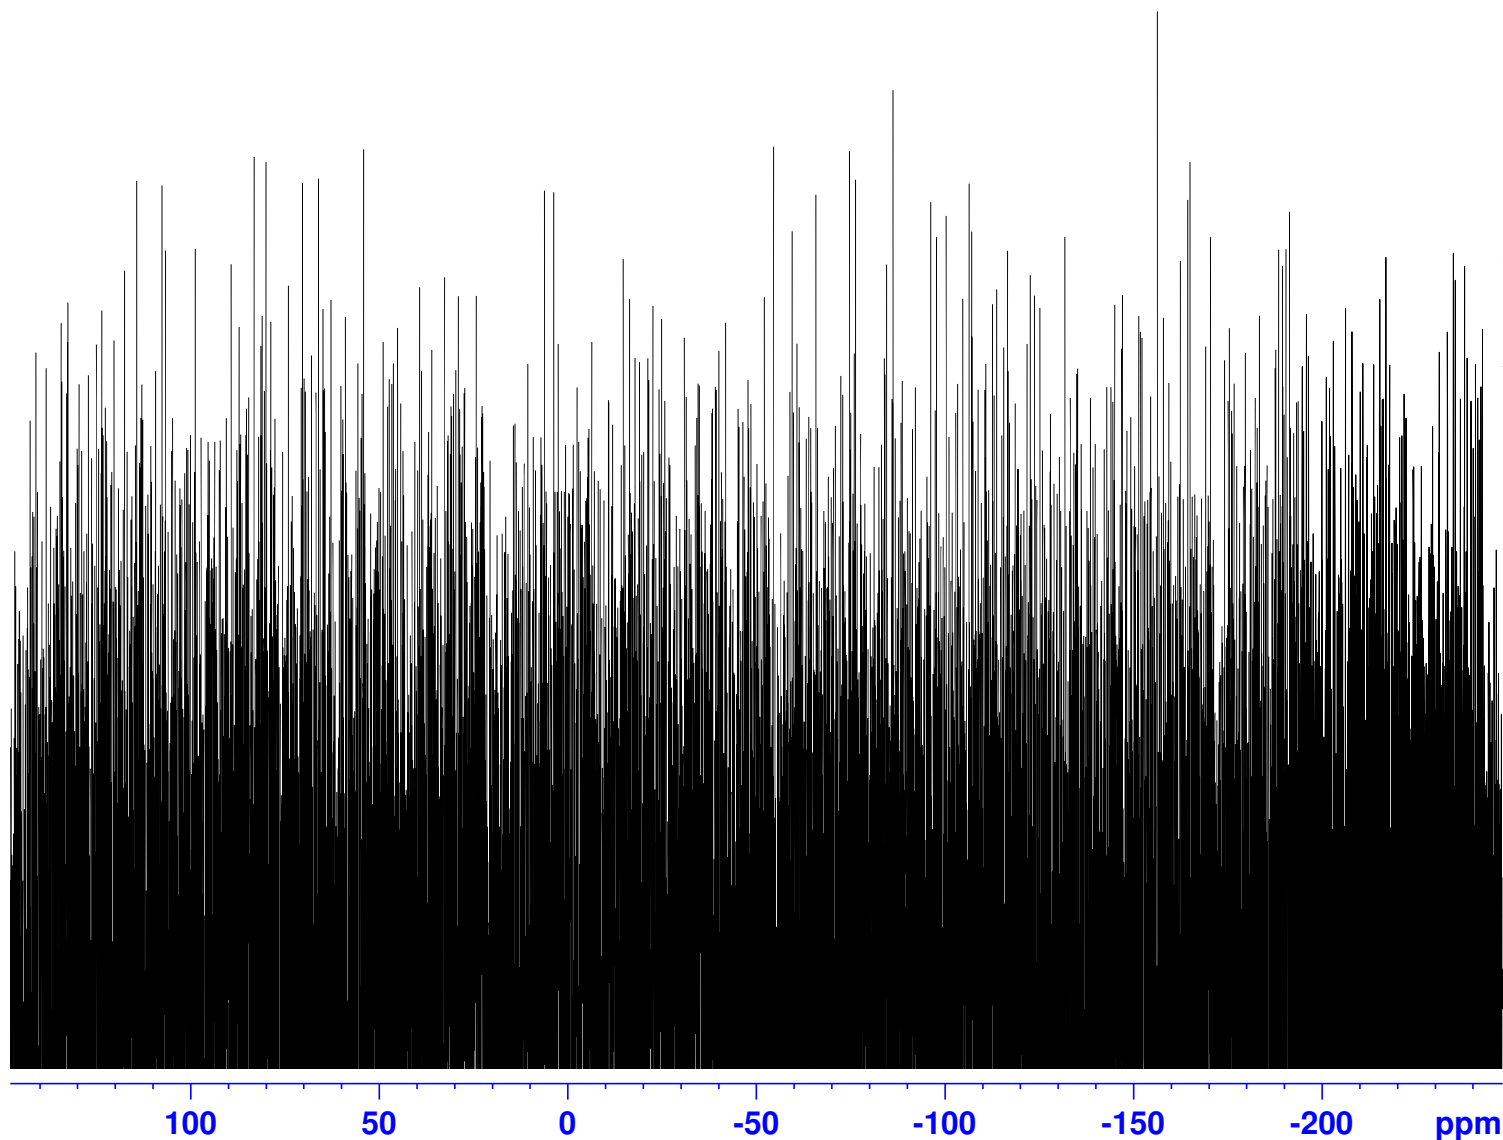

1.19
1.54
1.59
1.96
1.03
0.53
0.06
1.58
0.28
1.30
4.83
0.79
1.40
1.04
1.43
1.77
1.99
2.03
1.87
3.36
1.36
0.12
0.40
1.51
0.69
1.53
0.26
0.62
0.75
1.33
0.76
1.43
0.09
2.28
0.22
1.76
2.33
0.43
1.36
1.78
0.84
0.78
0.50
2.94
1.54
1.39