


FAHHEL COMP 1  
P31CPD CDC13 /opt/data Adv\_Exp 11

23.23

Current Data Parameters  
NAME X\_20190219  
EXPNO 62  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20190219  
Time 11.11 h  
INSTRUM spect  
PROBHD Z824801\_0046 (  
PULPROG zgpg30  
TD 65536  
SOLVENT CDC13  
NS 16  
DS 4  
SWH 64102.562 Hz  
FIDRES 1.956255 Hz  
AQ 0.5111808 sec  
RG 200.25  
DW 7.800 usec  
DE 6.50 usec  
TE 300.0 K  
D1 2.00000000 sec  
D11 0.03000000 sec  
TD0 1  
SFO1 162.0079729 MHz  
NUC1 31P  
P0 2.67 usec  
P1 8.00 usec  
PLW1 36.45100021 W  
SFO2 400.2316009 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 20.00000000 W  
PLW12 0.23714000 W  
PLW13 0.11928000 W

F2 - Processing parameters  
SI 32768  
SF 162.0160737 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40

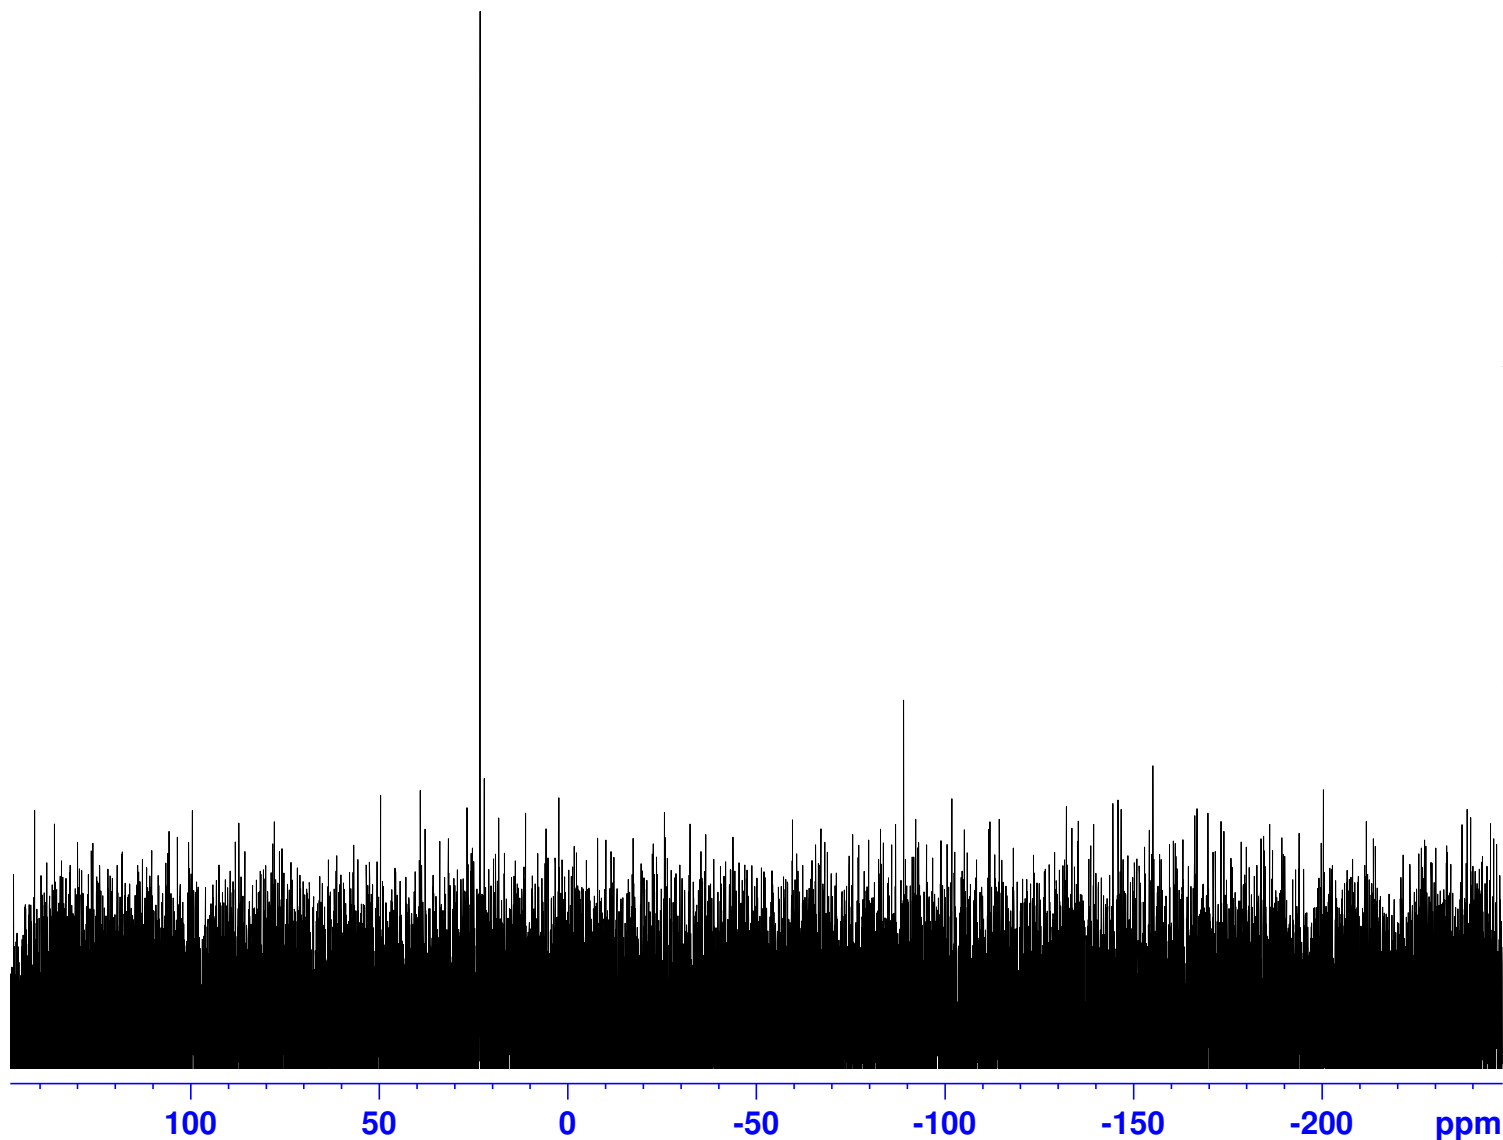

0.90  
1.04  
0.52  
0.30  
0.40  
0.92  
2.54  
0.71  
1.22  
0.48  
0.65  
1.84  
0.43  
1.42  
0.60  
1.50  
0.28  
1.17  
0.25  
1.11  
1.57  
0.85  
1.30  
0.01  
1.72  
0.55  
0.05  
2.34  
0.22  
0.16  
0.69  
1.30  
1.08  
0.29  
0.42  
0.85  
0.05  
0.90  
1.77  
0.30  
1.56  
1.49  
1.38  
0.39  
0.01  
1.13