


Angus pure 1
P31CPD CDC13 /opt/data Adv_Exp 5

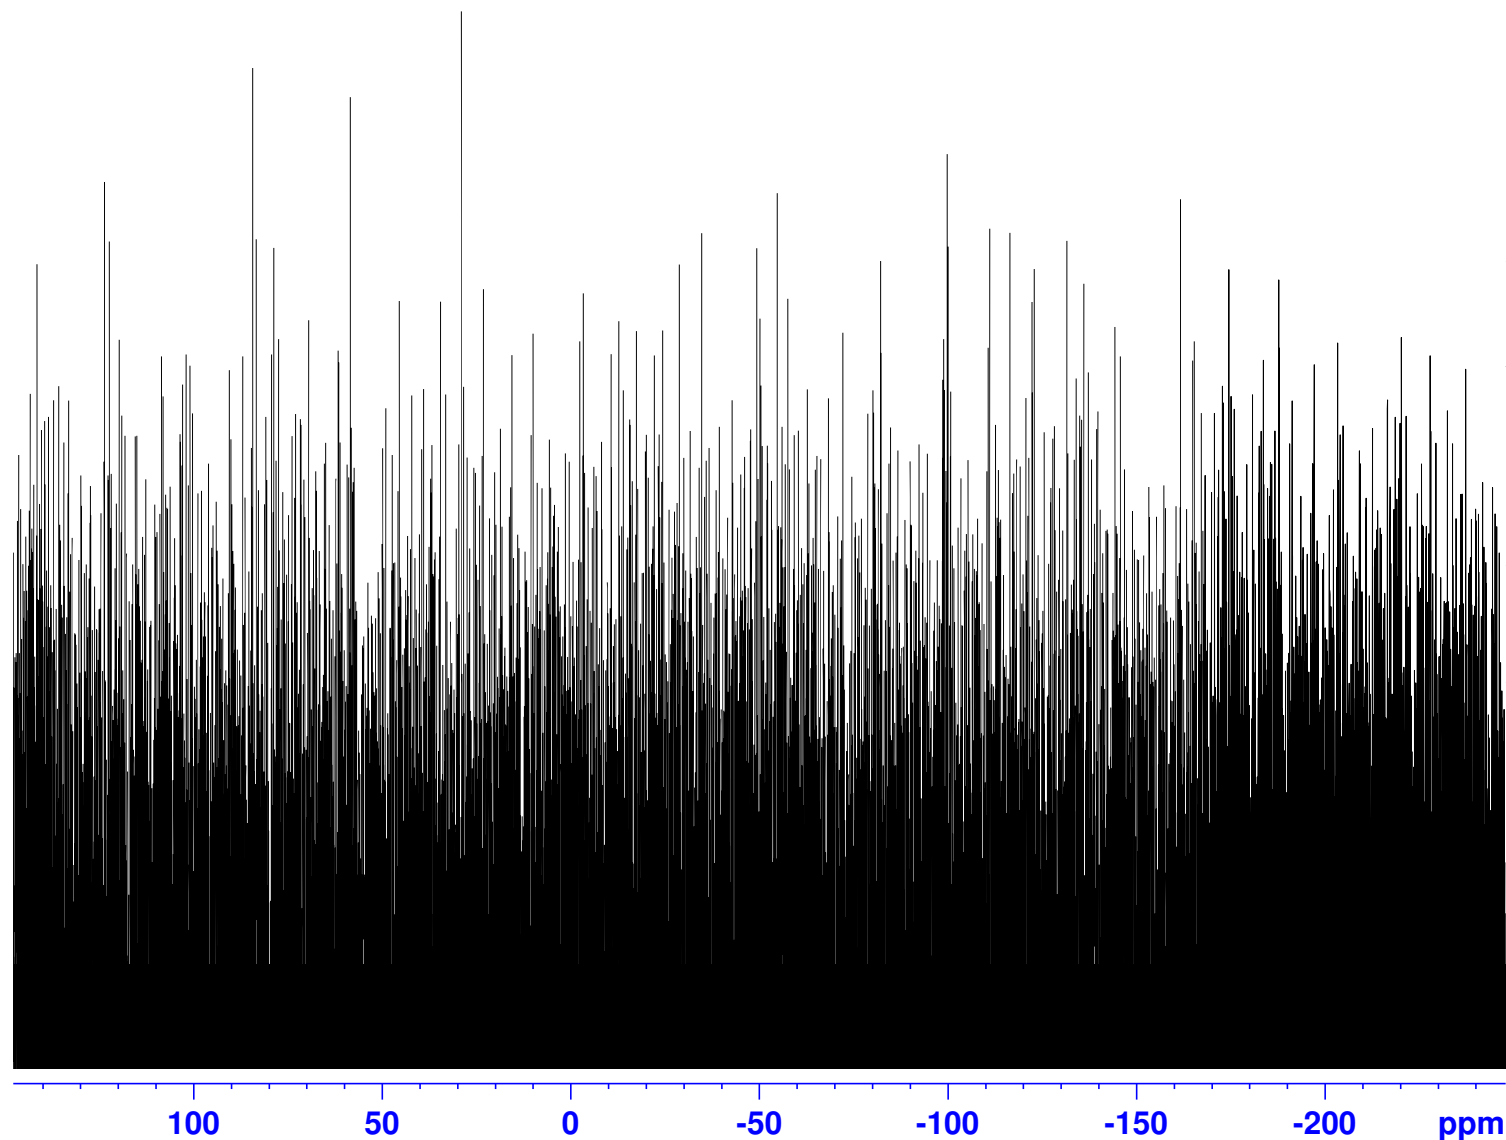

Current Data Parameters
NAME X_20190221
EXPNO 162
PROCNO 1

F2 - Acquisition Parameters
Date_ 20190221
Time 18.47 h
INSTRUM spect
PROBHD Z824801_0046 (
PULPROG zgpg30
TD 65536
SOLVENT CDC13
NS 16
DS 4
SWH 64102.562 Hz
FIDRES 1.956255 Hz
AQ 0.5111808 sec
RG 200.25
DW 7.800 usec
DE 6.50 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 162.0079729 MHz
NUC1 31P
P0 2.67 usec
P1 8.00 usec
PLW1 36.45100021 W
SFO2 400.2316009 MHz
NUC2 1H
CPDPRG2 waltz16
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.23714000 W
PLW13 0.11928000 W

F2 - Processing parameters
SI 32768
SF 162.0160737 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

0.64
1.73
0.83
2.04
0.10
0.17
0.58
1.77
1.36
0.34
1.73
0.69
0.94
0.50
0.67
1.02
1.06
0.12
0.10
0.32
1.45
1.47
0.59
2.55
0.72
0.94
0.44
1.27
0.08
0.81
3.08
1.17
1.01
1.79
1.21
1.14
0.17
0.36
0.73
0.58
0.06
2.77
0.77
0.82
0.91
0.82