


Nour Catalyst b take 2
P31CPD CDCl3 /opt/data Adv_Exp 22

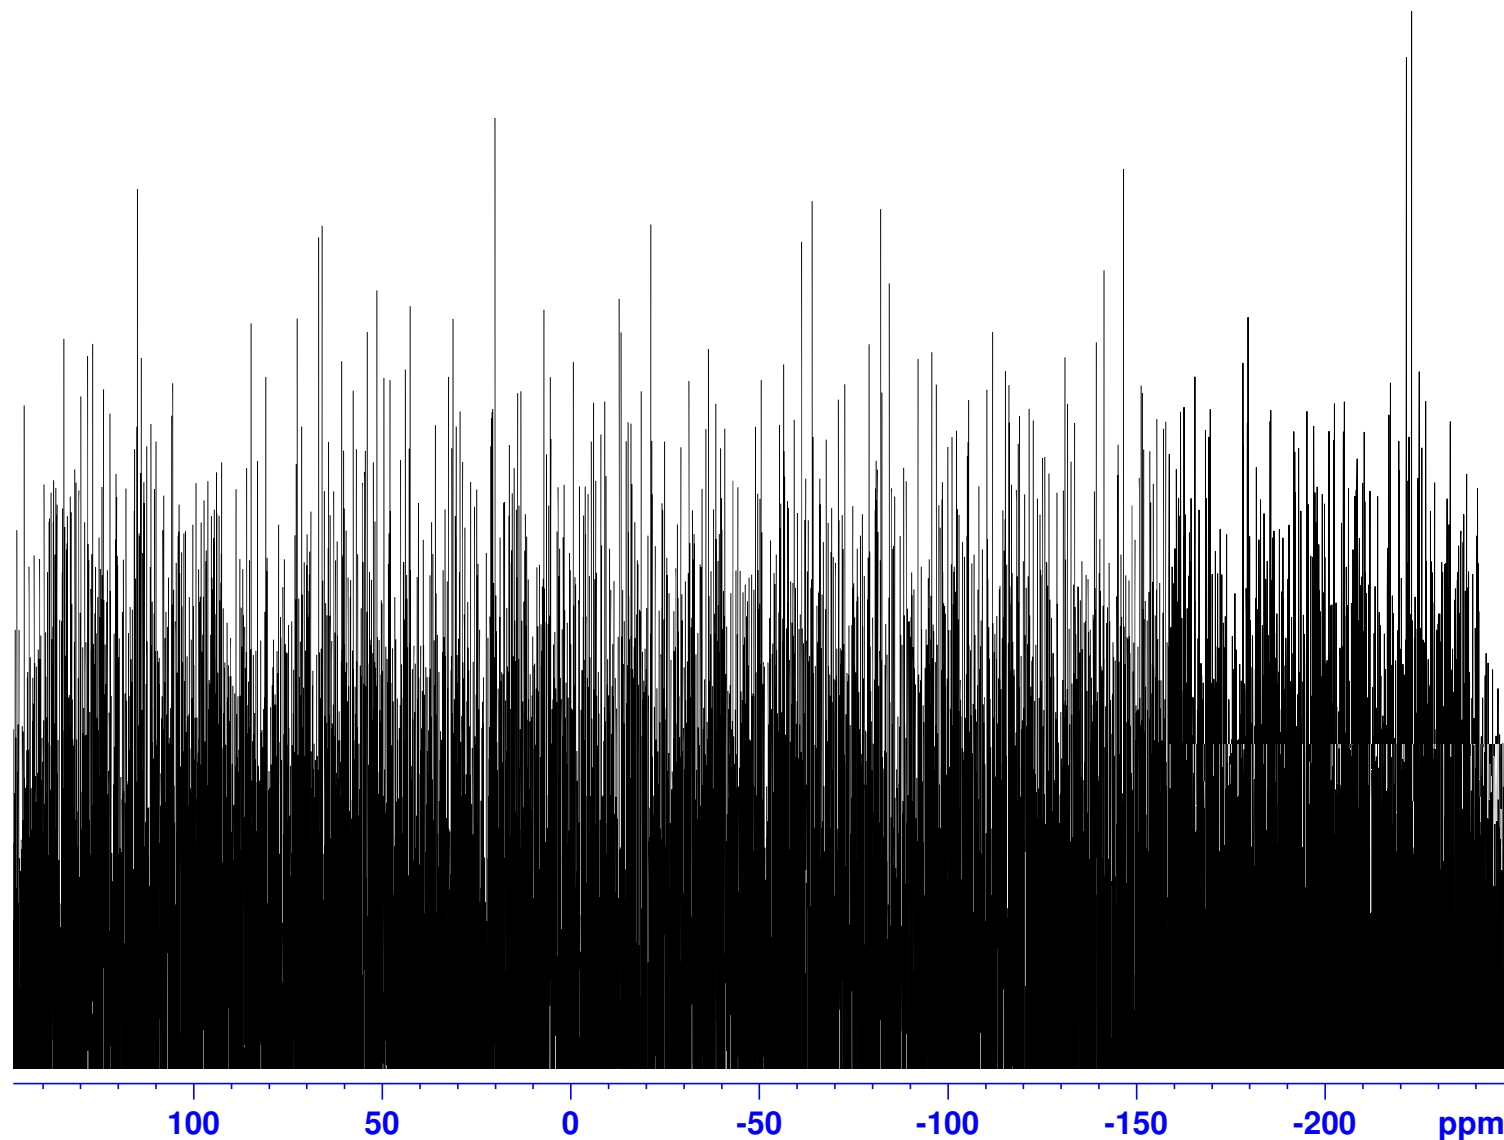

Current Data Parameters
NAME X_20190221
EXPNO 82
PROCNO 1

F2 - Acquisition Parameters
Date_ 20190221
Time 12.40 h
INSTRUM spect
PROBHD Z824801_0046 (
PULPROG zgpg30
TD 65536
SOLVENT CDCl3
NS 16
DS 4
SWH 64102.562 Hz
FIDRES 1.956255 Hz
AQ 0.5111808 sec
RG 200.25
DW 7.800 usec
DE 6.50 usec
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 162.0079729 MHz
NUC1 31P
P0 2.67 usec
P1 8.00 usec
PLW1 36.45100021 W
SFO2 400.2316009 MHz
NUC2 1H
CPDPRG2 waltz16
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.23714000 W
PLW13 0.11928000 W

F2 - Processing parameters
SI 32768
SF 162.0160737 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

0.87
1.43
0.48
0.47
1.30
2.36
1.63
2.08
1.13
0.66
0.53
2.42
0.58
0.55
0.53
1.34
2.55
2.34
0.33
0.88
1.38
0.96
0.88
2.77
0.85
1.06
2.12
2.37
1.91
1.25
1.00
1.82
1.64
1.51
0.13
0.41
2.44
1.17
1.92
1.49
1.18
1.35
0.26
1.34
0.23